


# Quality Assurance Manual

**TestAmerica West Sacramento**  
**880 Riverside Parkway**  
**West Sacramento, CA 95605**  
**Phone No. (916) 373-5600**  
**Fax No. (916) 372-1059**  
[www.testamericainc.com](http://www.testamericainc.com)

  
\_\_\_\_\_  
Laboratory Director – Karla Buechler

  
\_\_\_\_\_  
Date

  
\_\_\_\_\_  
Quality Manager - Pamela Schemmer

  
\_\_\_\_\_  
Date

**Copyright Information:**

This documentation has been prepared by TestAmerica Laboratories, Inc. and its affiliates (“TestAmerica”), solely for their own use and the use of their customers in evaluating their qualifications and capabilities in connection with a particular project. The user of this document agrees by its acceptance to return it to TestAmerica upon request and not to reproduce, copy, lend, or otherwise disclose its contents, directly or indirectly, and not to use if for any other purpose other than that for which it was specifically provided. The user also agrees that where consultants or other outside parties are involved in the evaluation process, access to these documents shall not be given to said parties unless those parties also specifically agree to these conditions.

**THIS DOCUMENT CONTAINS VALUABLE CONFIDENTIAL AND PROPRIETARY INFORMATION. DISCLOSURE, USE OR REPRODUCTION OF THESE MATERIALS WITHOUT THE WRITTEN AUTHORIZATION OF TESTAMERICA IS STRICTLY PROHIBITED. THIS UNPUBLISHED WORK BY TESTAMERICA IS PROTECTED BY STATE AND FEDERAL LAW OF THE UNITED STATES. IF PUBLICATION OF THIS WORK SHOULD OCCUR THE FOLLOWING NOTICE SHALL APPLY:**

©COPYRIGHT 2008 TESTAMERICA LABORATORIES, INC. ALL RIGHTS RESERVED

Facility Distribution No. \_\_\_\_\_

Distributed To: \_\_\_\_\_

**SECTION 2**  
**TABLE OF CONTENTS**

<b>Section No.</b>	<b>Title</b>	<b>Page No.</b>	<b>Effective Date</b>
1.0		COVER	5/16/2008
2.0	TABLE OF CONTENTS	2-1	5/16/2008
3.0	INTRODUCTION	3-1	1/1/2008
3.1	Introduction And Compliance References	3-1	1/1/2008
3.2	Terms And Definitions	3-1	1/1/2008
3.3	Scope / Fields Of Testing	3-2	1/1/2008
3.4	Management Of The Manual	3-2	1/1/2008
4.0	ORGANIZATION AND MANAGEMENT ( <i>NELAC 5.4.1</i> )	4-1	5/16/2008
4.1	Overview	4-1	5/16/2008
4.2	Roles And Responsibilities	4-2	5/16/2008
4.3	Deputies	4-9	5/16/2008
5.0	QUALITY SYSTEM ( <i>NELAC 5.4.2</i> )	5-1	1/1/2008
5.1	Quality Policy Statement	5-1	1/1/2008
5.2	Ethics And Data Integrity	5-1	1/1/2008
5.3	Quality System Supporting Documentation	5-2	1/1/2008
5.4	Qa/Qc Objectives For The Measurement Of Data	5-3	1/1/2008
5.5	Criteria For Quality Indicators	5-5	1/1/2008
5.6	Statistical Quality Control	5-5	1/1/2008
5.7	Quality System Metrics	5-6	1/1/2008
6.0	DOCUMENT CONTROL ( <i>NELAC 5.4.3</i> )	6-1	1/1/2008
6.1	Overview	6-1	1/1/2008
6.2	Document Approval And Issue	6-1	1/1/2008
6.3	Procedures For Document Control Policy	6-2	1/1/2008
6.4	Obsolete Documents	6-2	1/1/2008
7.0	REVIEW OF WORK REQUEST	7-1	1/1/2008
7.1	Overview	7-1	1/1/2008
7.2	Review Sequence And Key Personnel	7-2	1/1/2008
7.3	Documentation	7-3	1/1/2008
8.0	SUBCONTRACTING OF TESTS ( <i>NELAC 5.4.5</i> )	8-1	1/1/2008
8.1	Overview	8-1	1/1/2008
8.2	Qualifying And Monitoring Subcontractors	8-2	1/1/2008
8.3	Oversight And Reporting	8-5	1/1/2008
8.4	Contingency Planning	8-6	1/1/2008
9.0	PURCHASING SERVICES AND SUPPLIES ( <i>NELAC 5.4.6</i> )	9-1	5/16/2008
9.1	Overview	9-1	5/16/2008
9.2	Glassware	9-1	5/16/2008
9.3	Reagents, Standards & Supplies	9-1	5/16/2008
9.4	Purchase Of Equipment/Instruments/Software	9-3	5/16/2008
9.5	Services	9-4	5/16/2008

Section No.	Title	Page No.	Effective Date
9.6	Suppliers	9-4	5/16/2008
10.0	SERVICE TO THE CLIENT <i>(NELAC 5.4.7)</i>	10-1	1/1/2008
10.1	Overview	10-1	1/1/2008
10.2	Special Services	10-1	1/1/2008
10.3	Client Communication	10-1	1/1/2008
10.4	Reporting	10-1	1/1/2008
10.5	Client Surveys	10-2	1/1/2008
11.0	COMPLAINTS <i>(NELAC 5.4.8)</i>	11-1	1/1/2008
11.1	Overview	11-1	1/1/2008
11.2	External Complaints	11-1	1/1/2008
11.3	Internal Complaints	11-2	1/1/2008
11.4	Management Review	11-2	1/1/2008
12.0	CONTROL OF NON-CONFORMING WORK <i>(NELAC 5.4.9)</i>	12-1	1/1/2008
12.1	Overview	12-1	1/1/2008
12.2	Responsibilities And Authorities	12-1	1/1/2008
12.3	Evaluation Of Significance And Actions Taken	12-2	1/1/2008
12.4	Prevention Of Nonconforming Work	12-2	1/1/2008
12.5	Method Suspension/Restriction (Stop Work Procedures)	12-3	1/1/2008
13.0	CORRECTIVE ACTION <i>(NELAC 5.4.10)</i>	13-1	1/1/2008
13.1	Overview	13-1	1/1/2008
13.2	Definitions	13-1	1/1/2008
13.3	General	13-1	1/1/2008
13.4	Closed Loop Corrective Action Process	13-2	1/1/2008
13.5	Technical Corrective Actions	13-3	1/1/2008
13.6	Basic Corrections	13-3	1/1/2008
14.0	PREVENTIVE ACTION <i>(NELAC 5.4.11)</i>	14-1	1/1/2008
14.1	Overview	14-1	1/1/2008
15.0	CONTROL OF RECORDS <i>(NELAC 5.4.12)</i>	15-1	1/1/2008
15.1	Overview	15-1	1/1/2008
15.2	Technical And Analytical Records	15-4	1/1/2008
15.3	Laboratory Support Activities	15-5	1/1/2008
15.4	Administrative Records	15-6	1/1/2008
15.5	Records Management, Storage And Disposal	15-6	1/1/2008
16.0	AUDITS <i>(NELAC 5.4.13)</i>	16-1	5/16/2008
16.1	Overview	16-1	5/16/2008
16.2	Technical And Analytical Records	16-1	5/16/2008
16.3	External Audits	16-3	5/16/2008
16.4	Audit Findings	16-5	5/16/2008
17.0	MANAGEMENT REVIEWS <i>(NELAC 5.4.14)</i>	17-1	1/1/2008
17.1	Quality Assurance Report	17-1	1/1/2008
17.2	Annual Management Review	17-2	1/1/2008
17.3	Potential Integrity Related Managerial Reviews	17-3	1/1/2008
18.0	PERSONNEL <i>(NELAC 5.5.2)</i>	18-1	1/1/2008
18.1	Overview	18-1	1/1/2008

Section No.	Title	Page No.	Effective Date
18.2	Education And Experience Requirements For Technical Personnel	18-1	1/1/2008
18.3	Training	18-2	1/1/2008
18.4	Data Integrity And Ethics Training Program	18-3	1/1/2008
19.0	ACCOMMODATIONS AND ENVIRONMENTAL CONDITIONS (NELAC 5.5.3)	19-1	1/1/2008
19.1	Overview	19-1	1/1/2008
19.2	Environment	19-1	1/1/2008
19.3	Work Areas	19-2	1/1/2008
19.4	Floor Plan	19-2	1/1/2008
19.5	Building Security	19-3	1/1/2008
20.0	TEST METHODS AND METHOD VALIDATION (NELAC 5.5.4)	20-1	5/16/2008
20.1	Overview	20-1	5/16/2008
20.2	STANDARD OPERATING PROCEDURES (Sops)	20-1	5/16/2008
20.3	Laboratory Methods Manual	20-1	5/16/2008
20.4	Selection Of Methods	20-2	5/16/2008
20.5	Laboratory Developed Methods And Non-Standard Methods	20-5	5/16/2008
20.6	Validation Of Methods	20-6	5/16/2008
20.7	Method Detection Limits (Mdl)/ Limits Of Detection (Lod)	20-7	5/16/2008
20.8	Instrument Detection Limits (Idl)	20-9	5/16/2008
20.9	Verification Of Detection And Reporting Limits	20-9	5/16/2008
20.10	Retention Time Windows	20-9	5/16/2008
20.11	Evaluation Of Selectivity	20-10	5/16/2008
20.12	Estimation Of Uncertainty Of Measurement	20-10	5/16/2008
20.13	Control Of Data	20-11	5/16/2008
21.0	EQUIPMENT (AND CALIBRATIONS) (NELAC 5.5.5)	21-1	5/16/2008
21.1	Overview	21-1	5/16/2008
21.2	Preventive Maintenance	21-1	5/16/2008
21.3	Support Equipment	21-3	5/16/2008
21.4	Instrument Calibrations	21-5	5/16/2008
21.5	Policy On Tentatively Identified Compounds (Tics) – Gc/Ms Analysis	21-13	5/16/2008
21.6	Policy On Gc/Ms Tuning	21-13	5/16/2008
22.0	MEASUREMENT TRACEABILITY (NELAC 5.5.6)	22-1	5/16/2008
22.1	Overview	22-1	5/16/2008
22.2	Nist-Traceable Weights And Thermometers	22-2	5/16/2008
22.3	Reference Standards / Materials	22-2	5/16/2008
22.4	Documentation And Labeling Of Standards, Reagents, And Reference Materials	22-2	5/16/2008
23.0	SAMPLING (NELAC 5.5.7)	23-1	5/16/2008
23.1	Overview	23-1	5/16/2008
23.2	Sampling Containers	23-1	5/16/2008
23.3	Field Quality Control (Qc)	23-2	5/16/2008

Section No.	Title	Page No.	Effective Date
23.4	Definition Of Holding Time	23-2	5/16/2008
23.5	Sampling Containers, Preservation Requirements, Holding Times	23-3	5/16/2008
23.6	Sample Aliquots / Subsampling	23-3	5/16/2008
24.0	HANDLING OF SAMPLES <i>(NELAC 5.5.8)</i>	24-1	5/16/2008
24.1	Chain Of Custody (Coc)	24-1	5/16/2008
24.2	Sample Receipt	24-2	5/16/2008
24.3	Sample Acceptance Policy	24-3	5/16/2008
24.4	Sample Storage	24-3	5/16/2008
24.5	Hazardous Samples And Foreign Soils	24-3	5/16/2008
24.6	Sample Shipping	24-4	5/16/2008
24.7	Sample Disposal	24-4	5/16/2008
25.0	ASSURING THE QUALITY OF TEST RESULTS <i>(NELAC 5.5.9)</i>	25-1	5/16/2008
25.1	Overview	25-1	5/16/2008
25.2	Controls	25-1	5/16/2008
25.3	Negative Controls	25-1	5/16/2008
25.4	Positive Controls	25-2	5/16/2008
25.5	Sample Matrix Controls	25-4	5/16/2008
25.6	Acceptance Criteria (Control Limits)	25-6	5/16/2008
25.7	METHOD DETECTION LIMITS (Mdl's)	25-8	5/16/2008
25.8	Additional Procedures To Assure Quality Control	25-8	5/16/2008
26.0	REPORTING RESULTS <i>(NELAC 5.5.10)</i>	26-1	5/16/2008
26.1	Overview	26-1	5/16/2008
26.2	Test Reports	26-1	5/16/2008
26.3	Reporting Level Or Report Type	26-3	5/16/2008
26.4	Environmental Testing Obtained From <u>Subcontractors</u>	26-4	5/16/2008
26.5	Client Confidentiality	26-5	5/16/2008
26.6	Client Confidentiality	26-5	5/16/2008
26.7	Format Of Reports	26-6	5/16/2008
26.8	Amendments To Test Reports	26-6	5/16/2008
26.9	Policies On Client Requests For Amendments	26-6	5/16/2008

## LIST OF TABLES

Table No.	Title	Page	Effective Date
9-1	<u>Storage of Reagents and Chemicals</u>	9-5	5/16/2008
15-1	<u>Record Index</u>	15-1	1/1/2008
15-2	<u>Special Record Retention Requirements</u>	15-3	1/1/2008
16-1	<u>Audit Types and Frequency</u>	16-1	5/16/2008
21-1	<u>Example - Laboratory Equipment &amp; Instrumentation</u>	21-15	5/16/2008
21-2	<u>Example – Schedule of Routine Maintenance</u>	21-18	5/16/2008
21-3	<u>Example – Periodic Calibration</u>	21-25	5/16/2008
23-1	<u>Holding Times, Preservation and Container Requirements - Drinking Water (SDWA)</u>	23-5	5/16/2008
23-2	<u>Holding Times, Preservation and Container Requirements - NPDES – Bacteria, Protozoa, Toxicity Tests</u>	23-8	5/16/2008
23-3	<u>Holding Times, Preservation and Container Requirements - NPDES – Inorganic</u>	23-9	5/16/2008
23-4	<u>Holding Times, Preservation and Container Requirements - NPDES – Organic</u>	23-12	5/16/2008
23-5	<u>Holding Times, Preservation and Container Requirements - NPDES - Radiological</u>	23-14	5/16/2008
23-6	<u>Holding Times, Preservation and Container Requirements - RCRA – Aqueous</u>	23-15	5/16/2008
23-7	<u>Holding Times, Preservation and Container Requirements - RCRA – Non-Aqueous</u>	23-17	5/16/2008
23-8	<u>Holding Times, Preservation and Container Requirements - Air Samples</u>	23-19	5/16/2008

## LIST OF FIGURES

Figure No.	Title	Page	Effective Date
3-1	<u>Example - Format for a QA/QC Policy Memorandum</u>	3-4	1/1/2008
4-1	<u>Corporate Organizational Chart</u>	4-11	5/16/2008
8-1	<u>Example - Subcontracting Laboratory Approval Form (Initial / Renewal)</u>	8-7	1/1/2008
9-1	<u>Example - JD Edwards Vendor Add Request Form</u>	9-6	5/16/2008
13-1	<u>Example - Corrective Action Report</u>	13-5	1/1/2008
16-1	<u>Example - Internal Audit Workbook</u>	16-7	5/16/2008
16-2	<u>Example – Internal Audit System Checklist</u>	16-8	5/16/2008
17-1	<u>Example - QA Monthly Report to Management</u>	17-4	1/1/2008
17-2	<u>Example – Laboratory Metrics Categories</u>	17-6	1/1/2008
20-1	<u>Example – Demonstration of Capability Documentation</u>	20-19	5/16/2008
20-2	<u>Example – New Method / Additional Analyte Checklist</u>	20-20	5/16/2008
20-3	<u>Work Flow</u>	20-21	5/16/2008
24-1	<u>Example – Chain of Custody</u>	24-5	5/16/2008
24-2	<u>Example – Sample Acceptance Policy</u>	24-6	5/16/2008

## LIST OF APPENDICES

Appendix No.	Title	Page	Effective Date
1	<u>TestAmerica Ethics Policy No. CA-L-P-001</u>	Appendix 1-1	1/1/2008
2	<u>Example - Laboratory Organization Chart</u>	Appendix 2-1	5/16/2008
3	<u>Laboratory Floor Plan</u>	Appendix 3-1	1/1/2008
4	<u>Summary of Calibration, QC Procedures and Corrective Action</u>	Appendix 4-1	1/1/2008
5	<u>Glossary / Acronyms</u>	Appendix 5-1	1/1/2008
6	<u>Laboratory Certifications, Accreditations, Validations</u>	Appendix 6-1	1/1/2008
7	<u>Data Qualifiers</u>	Appendix 7-1	1/1/2008

## SOPs AND POLICIES REFERRED TO IN THE QA MANUAL

SOP/Policy Reference	Title
CA-Q-S-001	Solvent and Acid Lot Testing and Approval
CA-Q-S-002	Acceptable Manual Integration Practices
CA-Q-S-004	Method Compliance & Data Authenticity Audits
CA-Q-S-005	Calibration Curves (General)
CW-Q-S-001	Corporate Document Control and Archiving
CW-Q-S-002	Writing a Standard Operating Procedure (SOPs)
CA-L-S-001	Internal Investigation of Potential Data Discrepancies and Determination for Data Recall
CA-L-S-002	Subcontracting Procedures
CA-L-P-001	Ethics Policy
CA-L-P-002	Contract Compliance Policy
CW-L-P-001	Record Retention
CW-F-P-002	Authorization Matrix
CA-C-S-001	Work Sharing Process
CA-T-P-001	Qualified Products List
CW-F-S-004	Controlled Purchases Policy
WS-PQA-003	Quality Control Program
QA-012-SAC	Technical Data Review Requirements
S-ITQ-005	QuantIMS/JDE user Profile Setup and Maintenance
S-ITQ-007	Software Testing, Validation and Verification
WS-EHS-0001	Waste Disposal
SAC-PM-0004	Final Report Assembly and Third Level Data Review
WS-QA-0003	Sample Receipt and Procedures

<b>SOP/Policy Reference</b>	<b>Title</b>
SAC-QA-0004	Maintenance and Calibration Check of Fixed and Adjustable Volume Autopipettors, Autodispensers and Volumetric Containers
SAC-QA-0005	Temperature Monitoring and Corrective Action for Refrigerators and Freezers
SAC-QA-0006	Method Detection Limits (MDL) and Instrument Detection Limits (IDL)
SAC-QA-0007	Bottle and Cooler Preparation
SAC-QA-0016	Thermometer Calibration
WS-QA-0017	Standards and Reagents Preparation and Quality Control Check Procedures
SAC-QA-0022	Employee Orientation and Training
SAC-QA-0041	Calibration and Calibration Check of Balances
WS-QA-0009	Document Archiving
WS-PQA-013	Procedures to Address Customer Complaint
WS-QA-0018	Subsampling and Compositing of Samples (Method ASTM D 6323-98)
WS-QA-0021	Preparation and Management of SOPs
WS-QA-0023	NonConformance and Corrective Action System
WS-QA-0028	Multi-Incremental Subsampling of Soils and Sediments

## SECTION 3

### INTRODUCTION (NELAC 5.1 - 5.3)

#### 3.1 INTRODUCTION AND COMPLIANCE REFERENCES

TestAmerica West Sacramento's Quality Assurance Manual (QAM) is a document prepared to define the overall policies, organization objectives and functional responsibilities for achieving TestAmerica's data quality goals. Each TestAmerica laboratory maintains a local perspective in its scope of services and client relations and maintains a national perspective in terms of quality.

The QAM has been prepared to assure compliance with the 2003 National Environmental Laboratory Accreditation Conference (NELAC) standards and ISO/IEC Guide 17025 (1999). In addition, the policies and procedures outlined in this manual are compliant with the various accreditation and certification programs listed in Appendix 6. The relevant NELAC section is included in the heading of each QAM section.

The QAM has been prepared to be consistent with the requirements of the following documents:

- EPA 600/4-88/039, *Methods for the Determination of Organic Compounds in Drinking Water*, EPA, Revised July 1991.
- EPA 600/R-95/131, *Methods for the Determination of Organic Compounds in Drinking Water*, Supplement III, EPA, August 1995.
- EPA 600/4-79-019, *Handbook for Analytical Quality Control in Water and Wastewater Laboratories*, EPA, March 1979.
- EPA SW-846, *Test Methods for the Evaluation of Solid Waste*, 3<sup>rd</sup> Edition, September 1986; Update I, July 1992; Update II, September 1994; and Update III, December 1996.
- Federal Register, 40 CFR Parts 136, 141, 172, 173, 178, 179 and 261.
- USEPA Contract Laboratory Program, *Statement of Work for Inorganics Analysis, Multi-Media, Multi-Concentration*. Document ILM04.0.
- USEPA Contract Laboratory Program, *Statement of Work for Organics Analysis, Multi-Media, Multi-Concentration*. Document Number OLM03.1, August 1994.
- APHA, *Standard Methods for the Examination of Water and Wastewater*, 18<sup>th</sup> Edition, 19<sup>th</sup>, 20<sup>th</sup> and 21<sup>st</sup> Edition.
- U.S. Department of Defense, *Quality Systems Manual for Environmental Laboratories*, Final Version 3, January 2006.
- U.S. Department of Defense, *Air Force Center for Environmental Excellence Quality Assurance Project Plan (QAPP)*, Version 4.0.02, May 2006.

#### 3.2 TERMS AND DEFINITIONS

A Quality Assurance Program is a company-wide system designed to ensure that data produced by TestAmerica West Sacramento conforms to the standards set by state and/or federal regulations. The program functions at the management level through company goals and management policies, and at the analytical level through Standard Operating Procedures (SOPs) and quality control. The TestAmerica program is designed to minimize systematic error,

encourage constructive, documented problem solving, and provide a framework for continuous improvement within the organization.

Refer to Appendix 5 for the Glossary/Acronyms.

### **3.3 SCOPE / FIELDS OF TESTING**

TestAmerica West Sacramento analyzes thousands of environmental and industrial samples every month. Sample matrices vary among air, drinking water, effluent water, groundwater, hazardous waste, sludge, soils, and biological tissues. The Quality Assurance Program contains specific procedures and methods to test samples of differing matrices for chemical, physical and biological parameters. The Program also contains guidelines on maintaining documentation of analytical process, reviewing results, servicing clients and tracking samples through the laboratory. The technical and service requirements of all requests to provide analyses are thoroughly evaluated before commitments are made to accept the work. Measurements are made using published reference methods or methods developed and validated by the laboratory.

The methods covered by this manual include the most frequently requested water, air, industrial waste, and soil methodologies needed to provide analytical services in the United States, its territories, and foreign countries. The specific list of test methods used by the laboratory can be found in Appendix 4 of this document. The approach of this manual is to define the minimum level of quality assurance and quality control necessary to meet requirements. All methods performed by TestAmerica West Sacramento shall meet these criteria as appropriate. In some instances, quality assurance project plans (QAPPs), project specific data quality objectives (DQOs) or local regulations may require criteria other than those contained in this manual. In these cases, the laboratory will abide by the requested criteria following review and acceptance of the requirements by the Laboratory Director or the Quality Assurance (QA) Manager. In some cases, QAPPs and DQOs may specify less stringent requirements. The Laboratory Director and the QA Manager must determine if it is in the lab's best interest to follow the less stringent requirements.

### **3.4 MANAGEMENT OF THE MANUAL**

#### **3.4.1 Review Process**

The manual is reviewed annually by the QA Manager and laboratory personnel to assure that it reflects current practices and meets the requirements of TestAmerica West Sacramento's clients and regulators. Occasionally, the manual may need changes in order to meet new or changing regulations and operations. The QA Manager will review the changes in the normal course of business and incorporate changes into revised sections of the document. The updates will be reviewed by the QA Manager, Laboratory Director, Technical Director(s), relevant operational staff and Corporate Quality Assurance (if a change is made to the Corporate template) and then formally incorporated into the document in periodic updates. The QAM is based on a Corporate QAM Template that is prepared and approved by the Chief Operating Officers (COOs) and Corporate Quality Assurance. This template is reviewed annually by the COOs, Corporate Quality, and each laboratory. Necessary changes are coordinated by the Vice President of Quality and Environmental Health & Safety (EHS) and distributed to each laboratory for inclusion in the laboratory specific QA Manuals.

Policies in the QAM that require immediate attention may be addressed through the use of Corporate QA/QC Policy Memoranda. QA/QC Policy Memoranda are published from time to time to facilitate immediate changes to QA/QC Policy. QA/QC Policy Memoranda supersede the QAM and all other SOPs (refer to Section 5.3). All policy memoranda are dated, archived and distributed by their placement into the front of the QAM between the signature page and Section 2. At a minimum, each policy memorandum is approved by the same authorized signatories as shown on the cover page of the QA Manual. In addition, Corporate QA/QC Policy Memoranda are signed by the COOs and VP of Quality and EHS. The QA/QC Policy Memoranda are incorporated into the QAM during the periodic updates. Policy memorandum may also include an expiration date if appropriate. An example format can be found in Figure 3-1. A similar procedure is followed for local laboratory changes.

Laboratory-specific QAM changes are approved and documented according to the laboratory SOP WS-QA-0021, "Preparation and Management of Standard Operating Procedures".

### **3.4.2 Control**

This manual is considered confidential within TestAmerica and may not be altered in any manner by other than a duly appointed representative from TestAmerica. If the document has been provided to external users or regulators, it is for the exclusive purpose of reviewing TestAmerica West Sacramento's quality systems and shall not be used in any other way without the written permission of an appointed representative of TestAmerica. The procedure for control of distribution is incorporated by reference to the laboratory SOP WS-QA-0021, "Preparation and Management of Standard Operating Procedures".

The order of precedence in the event of a conflict between policies is outlined in Section 5.3 of this Quality Assurance Manual.

**Figure 3-1.**

**Example - Format for a QA/QC Policy Memorandum**

**Corporate (or Laboratory) QA/QC Policy Memorandum # \_\_\_\_\_**

Effective Date: \_\_\_\_\_ Expiration Date: When Appropriate QAM Section is Revised

<b>Corporate:</b> <i>(Only needed for Corporate Memorandum – Delete if Laboratory)</i>			
_____ COO - West	_____ Date	_____ Vice-President, QA and EHS	_____ Date
_____ COO - East	_____ Date		
<b>Local:</b>			
_____ Laboratory Director Approval	_____ Date	_____ Quality Assurance Approval	_____ Date

1. **Purpose**
2. **Procedure**
3. **Attachments**
4. **References/Cross References**

## SECTION 4

### ORGANIZATION AND MANAGEMENT (NELAC 5.4.1)

#### 4.1 OVERVIEW

TestAmerica West Sacramento is part of a national network of laboratories known as TestAmerica. This Quality Assurance Manual (QAM) is applicable to the TestAmerica West Sacramento laboratory only.

TestAmerica West Sacramento  
880 Riverside Parkway  
West Sacramento, CA 95605  
EPA ID CA00044

The Corporate organization chart can be found in Figure 4-1 and the laboratory's organization chart can be found in Appendix 2. The locations of other TestAmerica labs are as follows:

TestAmerica Anchorage  
TestAmerica Austin  
TestAmerica Buffalo  
TestAmerica Buffalo Grove  
TestAmerica Burlington  
TestAmerica Cedar Falls  
TestAmerica Chicago  
TestAmerica Connecticut  
TestAmerica Corpus Christi  
TestAmerica Dayton  
TestAmerica Denver  
TestAmerica Edison  
TestAmerica Honolulu  
TestAmerica Houston  
TestAmerica Irvine  
TestAmerica King of Prussia  
TestAmerica Knoxville  
TestAmerica Los Angeles  
TestAmerica Mobile  
TestAmerica Morgan Hill  
TestAmerica Nashville  
TestAmerica North Canton  
TestAmerica Ontario  
TestAmerica Orlando  
TestAmerica Pensacola  
TestAmerica Phoenix  
TestAmerica Pittsburgh  
TestAmerica Portland  
TestAmerica Richland

TestAmerica San Francisco  
TestAmerica Savannah  
TestAmerica Seattle  
TestAmerica Spokane  
TestAmerica St. Louis  
TestAmerica Tacoma  
TestAmerica Tallahassee  
TestAmerica Tampa  
TestAmerica Valparaiso  
TestAmerica Watertown  
TestAmerica Westfield

## **4.2 ROLES AND RESPONSIBILITIES**

In order for the Quality Assurance Program to function properly, all members of the staff must clearly understand and meet their individual responsibilities as they relate to the quality program. The following descriptions define each role in its relationship to the Quality Assurance Program. More extensive job descriptions are maintained on the laboratory intranet site OASIS.

### **4.2.1 Quality Assurance Program**

The responsibility for quality lies with every employee of TestAmerica West Sacramento. All employees have access to the QAM and are responsible for knowing the content of this manual and upholding the standards therein. Each person carries out his/her daily tasks in a manner consistent with the goals and in accordance with the procedures in this manual and the laboratory's SOPs.

### **4.2.2 President/Chief Executive Officer (CEO)**

The President/CEO is a member of the Board of Directors and is ultimately responsible for the quality and performance of all TestAmerica facilities. The President/CEO establishes the overall quality standard and data integrity program for the Analytical Division, providing the necessary leadership and resources to assure that the standard and integrity program are met.

### **4.2.3 Chief Operating Officer (COO)**

The COO serves as the ranking executive for all respective analytical laboratory operational functions and reports to the President/CEO of the Analytical Division. The COO is responsible for the daily management of all analytical laboratories, long-term planning and development of technical policies and management plans. The COO ensures the attainment of corporate objectives through the selection, development, motivation, and evaluation of top management personnel. The COO approves all operating budgets and capital expenditures. The COO signs-off on the final QAM template that contains company policies for implementing the Quality Program.

### **4.2.4 General Manager (GM)**

Each GM reports directly to a COO. Each GM has full responsibility for the overall administrative and operational management of their respective laboratories. The GM's responsibilities include allocation of personnel and resources, long-term planning, setting goals,

and achieving the financial, business, and quality objectives of TestAmerica. The GM ensures timely compliance with corporate management directives, policies, and management systems reviews. The GM is also responsible for restricting any laboratory from performing analyses that cannot be consistently and successfully performed to meet the standards set forth in this manual.

#### **4.2.5 Vice President of Client and Technical Services**

The Vice President (VP) of Client and Technical Services reports directly to the President/CEO and is responsible for offerings to clients including quality assurance, environmental health and safety, risk management, technical assistance, legal compliance and contract administration. The VP of Client and Technical Services provides support and direction to the Executive Director and Directors of these areas, and supports the COO in decisions regarding long term planning, resource allocation and capital expenditures.

#### **4.2.6 Executive Director of Quality and Environmental Health and Safety (QA/EHS)**

The Executive Director of QA/EHS reports to the VP of Client and Technical Services. With the aid of the Senior Management Team, Laboratory Director/ Managers, Quality Directors, EHS Directors, QA Managers and EHS Coordinators, the Executive Director-QA/EHS has the responsibility for the establishment, general overview and Corporate maintenance of the Quality Assurance and Environmental, Health and Safety Program within TestAmerica. Additional responsibilities include:

- Review of QA/QC aspects of Corporate SOPs, national projects and expansions or changes in services.
- Coordination/preparation of the Corporate QAM Template that is used by each laboratory to prepare its own laboratory-specific QAM.
- Maintenance of Corporate Policies, Quality Memorandums and SOPs. Maintenance of data investigation records that are reported to Corporate Management.
- Working with various organizations outside of TestAmerica to further the development of quality standards and represent TestAmerica at various trade meetings.
- Preparation of a monthly report that includes quality metrics across the Analytical Division and a summary of any quality related initiatives and issues.
- With the assistance of the Corporate Senior Management Team and the EHS Directors, development and implementation of the TestAmerica Environmental, Health and Safety Program.

#### **4.2.7 Quality Directors (Corporate)**

The Quality Directors report to the Executive Director-QA/EHS. Together with the Executive Director-QA/EHS, the Quality Directors have the responsibility for the establishment, general overview and maintenance of the Analytical Division's Quality Assurance Program within TestAmerica. The Quality Directors are responsible for:

- Oversight of the QA/QC programs within each laboratory. This includes a final review of each laboratory-specific QAM and receipt of each laboratory's QA monthly report.

- Working with management to develop a plan of correction when a laboratory's quality system is determined to be inadequate.
- Review of QA/QC aspects of national projects.
- Assistance with certification activities.
- Providing assistance as needed in the selection of Quality Assurance Managers and reviewing their effectiveness.

#### **4.2.8 Ethics and Compliance Officers (ECOs)**

TestAmerica has designated two senior members of the Corporate staff to fulfill the role of Ethics and Compliance Officer (ECO) – VP-Client and Technical Services and the Executive Director–QA/EHS. Each ECO acts as a back-up to the other ECO and both are involved when data investigations occur. Each ECO has a direct line of communication to the entire senior Corporate and lab management staff.

The ECOs ensure that the organization distributes the data integrity and ethical practices policies to all employees and ensures annual trainings and orientation of new hires to the ethics program and its policies. The ECO is responsible for establishing a mechanism to foster employee reporting of incidents of illegal, unethical, or improper practices in a safe and confidential environment.

The ECOs monitor and audit procedures to determine compliance with policies and to make recommendations for policy enhancements to the CEO, COO, Laboratory Director/Manager or other appropriate individuals within the laboratory. The ECO will assist the laboratory QA Manager in the coordination of internal auditing of ethical policy related activities and processes within the laboratory, in conjunction with the laboratories regular internal auditing function.

The ECOs will also participate in investigations of alleged violations of policies and work with the appropriate internal departments to investigate misconduct, remedy the situation, and prevent recurrence of any such activity.

#### **4.2.9 Director of Technical Services**

The Director of Technical Services is responsible for establishing, implementing and communicating TestAmerica's Technical Policies, SOPs, and Manuals. Other responsibilities include conducting technical assessments as required, acting as a technical resource in national contracts review, coordinating new technologies, establishing best practices, advising staff on technology advances, innovations, and applications.

#### **4.2.10 Chief Information Officer (CIO)**

The CIO is responsible for establishing, implementing and communicating TestAmerica's Information Technology (IT) Policies, SOPs and Manuals. Other responsibilities include coordinating new technologies, development of electronic communication tools such as TestAmerica's intranet and internet sites, ensuring data security and documentation of software, ensuring compliance with the NELAC standard, and assistance in establishing, updating, and

maintaining Laboratory Information Management Systems (LIMS) at the various TestAmerica facilities.

#### **4.2.11 Environmental Health and Safety Directors (EHSDs) (Corporate)**

The EHSDs report directly to the Executive Director-QA/EHS. The EHSDs are responsible for the development and implementation of the TestAmerica Environmental, Health and Safety program. Responsibilities include:

- Consolidation and tracking all safety and health-related information and reports for the company, and managing compliance activities for TestAmerica locations.
- Coordination/preparation of the corporate Environmental, Health and Safety Manual Template that is used by each laboratory to prepare its own laboratory-specific Safety Manual/CHP.
- Development and execution of the company Environmental Health and Safety Internal Audit program.
- Preparation of information and training materials for laboratory EHS Coordinators.
- Assistance in the internal and external coordination of employee exposure and medical monitoring programs to insure compliance with applicable safety and health regulations.
- Serving as Department of Transportation (D.O.T.) focal point and providing technical assistance to location management.
- Serving as Hazardous Waste Management main contact and providing technical assistance to location management.

#### **4.2.12 Laboratory Director / Technical Director**

TestAmerica West Sacramento's Laboratory Director is responsible for the overall quality, safety, financial, technical, human resource and service performance of the whole laboratory and reports to their respective GM. The Laboratory Director provides the resources necessary to implement and maintain an effective and comprehensive Quality Assurance and Data Integrity Program.

Specific responsibilities include, but are not limited to:

- Reports directly to the General Manager
- Responsible for implementation and adherence by lab staff to the TestAmerica West Sacramento QAM and all policies and procedures within the laboratory
- Has signature authority for LQM, policies, SOPs, and contracts (as detailed in TestAmerica policy)
- Annually assesses the effectiveness of the QMP and LQM within the operation
- Maintains adequately trained staff documented on organization charts
- Responsible for implementing internal/external audit findings corrective actions.

#### **4.2.13 Quality Assurance (QA) Manager**

The QA Manager has responsibility and authority to ensure the continuous implementation of the quality system based on ISO 17025.

The QA Manager reports directly to the Laboratory Director and has access to Corporate QA for advice and resources. This position is able to evaluate data objectively and perform assessments without outside (i.e., managerial) influence. Corporate QA may be used as a resource in dealing with regulatory requirements, certifications and other quality assurance related items. The QA Manager directs the activities of the QA department to accomplish specific responsibilities, which include, but are not limited to:

- Reports directly to the Laboratory Director and, for all QA matters, to the Corporate QA Director to maintain independence of QA oversight
- Responsible for implementing and communicating the QMP
- Maintains, approves, and implements the QAM
- Has joint signature authority, with the Laboratory Director, for approval of quality documents, e.g., QAM, policies, and SOPs
- Directs controlled distribution of laboratory quality documents
- Provides Quality System training to all new personnel
- Reviews and approves documentation of analyst training records
- Serves as a focal point for QA and QC issues, reviews corrective actions and recommends resolution for recurring nonconformances within the laboratory
- Assists in maintaining regulatory analytical compliance, including maintaining certifications, and in this regard has signature authority for laboratory quality documents
- Monitors data quality measures via statistical methods to verify that the laboratory routinely meets stated quality goals
- Performs systems, data, contract compliance, and surveillance audits
- Hosts external audits conducted by outside agencies
- Responsible for approving quality control reference data changes in the LIMS
- Oversees the selection, review, and approval of analytical subcontractors
- Prepares monthly QA Reports to management describing significant quality events
- Has the final authority to accept or reject data and to stop work in progress in the event that procedures or practices compromise the validity and integrity of analytical data.

#### **4.2.14 Operations Manager/Technical Director**

- Reports directly to the Laboratory Director
- Supervises daily activities of the Operational Groups
- Schedules analytical operations
- Supervises QC activities performed as a part of routine analytical operations
- Implements data review procedures

- Supervises the preparation and maintenance of laboratory records
- Supervises maintenance of instruments and scheduling of repairs
- Works with the Project Managers and Group/Team Leaders to assure the requirements of projects are met in a timely manner
- Responsible for meeting quality requirements
- Responsible for the technical operation of the laboratory  
Responsible for coordinating the development and implementation of SOPs
- Performs technical training in area(s) of expertise
- Interfaces with management on technical needs and solving day-to-day technical issues
- Determines qualifications required for technical positions and evaluates job candidates against those requirements
- Investigates technical issues related to projects as directed by QA
- Evaluates new methods, technical proposals, and statements of work
- Certifies technical laboratory personnel based on education and background to ensure that staff have demonstrated capability in the activities for which they are responsible  
Performs other tasks as required by NELAC.
- The Technical Director meets the requirements specified in the Section 4.1.1.1 of the NELAC standards.

#### **4.2.15 Manager of Customer Services**

- Reports directly to the Laboratory Director
- Supervises daily activities of the Project Management, and/or Sample Control, and/or Administrative, and/or Report Production Groups
- Works with the Operations Manager and/or Department Managers to ensure the requirements of projects are met in a timely manner
- Has signature authority for contracts for laboratory services, as detailed in TestAmerica policy, and for laboratory reports.
- Defines customer requirements through project definition
- Assesses and assures customer satisfaction
- Provides feedback to management on changing customer needs
- Brings together resources necessary to ensure customer satisfaction.

#### **4.2.16 Project Manager**

- Reports directly to the Manager of Customer Service or Project Management Department Manager
- Monitors analytical and QA project requirements for a specified project
- Acts as a liaison between the client and the laboratory staff
- Prepares Quality Assurance Summary (QAS) or equivalent summary form and communicates project-specific requirements to all parties involved

- Assists the laboratory staff with interpretation of work plans, contracts, and QAPP requirements
- Reviews project data packages for completeness and compliance with client needs
- Has signature authority for final reports
- Keeps the laboratory and client informed of project status
- Together with the QA Manager, approves customer requested variances to methods and to standard laboratory protocols
- Monitors, reviews, and evaluates the progress and performance of projects
- Reports client inquiries involving data quality issues or data acceptability to the facility QA Manager and to the operations staff
- Prepares reissue requests for project data
- Responsible for meeting quality requirements.

#### **4.2.17 Project Administrator**

- Reports directly to the Manager of Customer Service or Project Management Department Manager
- Monitors analytical and QA project requirements for a specified project
- Acts as a liaison between the client and the laboratory staff
- Prepares Quality Assurance Summary (QAS) or equivalent summary form and communicates project-specific requirements to all parties involved
- Assists the laboratory staff with interpretation of work plans, contracts, and QAPP requirements
- Reviews project data packages for completeness and compliance with client needs
- Keeps the laboratory and client informed of project status
- Together with the QA Manager, approves customer requested variances to methods and to standard laboratory protocols
- Monitors, reviews, and evaluates the progress and performance of projects
- Reports client inquiries involving data quality issues or data acceptability to the facility QA Manager and to the operations staff
- Prepares reissue requests for project data
- Responsible for meeting quality requirements.

#### **4.2.18 Department Manager, Team Leader, or Supervisor**

- Reports directly to the Operations Manager
- Supervises daily activities of analyses within the group
- Supervises QC activities performed as a part of routine analytical operations
- Implements data review procedures
- Supervises the preparation and maintenance of laboratory records

- Evaluates instrument performance and supervises the calibration, preventive maintenance, and scheduling of repairs
- Oversees or performs review and approval of all analytical data
- Reports nonconformances to the appropriate managers
- Responsible for generation of SOPs for their section
- Responsible for meeting quality requirements.

**4.2.19 Analyst**

- Performs analytical methods and data recording in accordance with documented procedures
- Performs and documents calibration and preventive maintenance
- Performs data processing and data review procedures
- Reports nonconformances to the Supervisor/Manager and QA Manager
- Ensures sample and data integrity by adhering to internal chain-of-custody procedures
- Responsible for meeting quality requirements defined in this LQM and other supporting QA procedures.
- 

**4.2.20 Sample Custodian**

- Ensures implementation of proper sample receipt procedures, including maintenance of chain-of-custody
- Reports nonconformances associated with condition-upon-receipt of samples
- Logs samples into the LIMS
- Ensures that all samples are stored in the proper environment
- Assists Environmental Health and Safety staff with sample disposal
- Responsible for meeting quality requirements.

**4.2.21 Report Production Staff**

- Accurately generates and compiles analytical reports and associated deliverables for delivery to the client
- Responsible for meeting quality requirements
- Produce, as needed, reports that meet the NELAC requirements.

**4.3 DEPUTIES**


The following table defines who assumes the responsibilities of key personnel in their absence:

Key Personnel	Deputy	Comment
Laboratory Director	Technical Director of Air Toxics/Deputy Laboratory Technical Director Or Manager of Operations/Deputy	

Key Personnel	Deputy	Comment
	Laboratory Technical Director	
QA Manager	Laboratory Director or Quality Assurance Scientist	

Figure 4-1.

Corporate Organization Chart

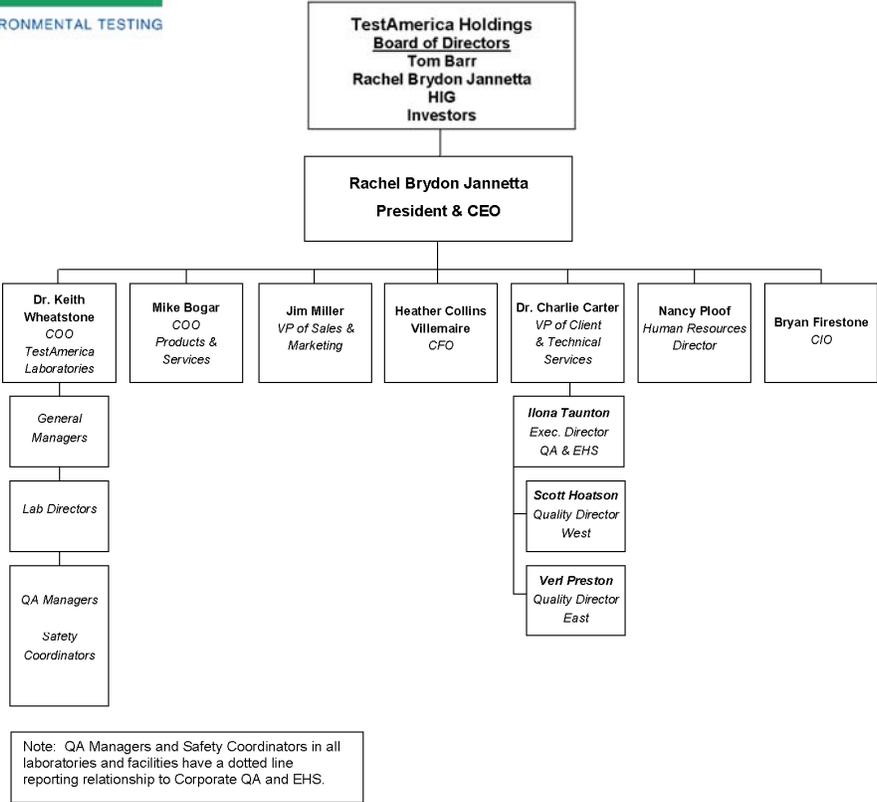

## SECTION 5

### QUALITY SYSTEM (NELAC 5.4.2)

#### 5.1 QUALITY POLICY STATEMENT

The management of TestAmerica and TestAmerica West Sacramento are committed to providing data of known quality to its clients by adhering to approved methodologies, regulatory requirements and the QA/QC protocols described in this manual.

In all aspects of the laboratory and business operations, management is dedicated in maintaining the highest ethical standards. An Ethics Policy sign-off can be viewed in Appendix 1. Training on ethical and legal responsibilities is provided annually and each employee signs off annually on the policy as a condition of employment.

It is TestAmerica's Policy to continually improve systems and provide support to quality improvement efforts in laboratory, administrative and managerial activities. The company recognizes that the implementation of a quality assurance program requires management's commitment and support as well as the involvement of the entire staff.

TestAmerica West Sacramento strives to provide clients with the highest level of professionalism and the best service practices in the industry.

Every staff member at TestAmerica West Sacramento plays an integral part in quality assurance and is held responsible and accountable for the quality of their work. It is, therefore, required that all laboratory personnel are trained and agree to comply with applicable procedures and requirements established by this document.

#### 5.2 ETHICS AND DATA INTEGRITY

TestAmerica is committed to ensuring the integrity of its data and meeting the quality needs of its clients. The 7 elements of TestAmerica's Ethics and Data Integrity Program include:

- An Ethics Policy (Policy No. CA-L-P-001) and employee ethics statements (Appendix 1).
- An Ethics and Compliance Officer (ECO).
- A training program.
- Self-governance through disciplinary action for violations.
- A confidential mechanism for anonymously reporting alleged misconduct and a means for conducting internal investigations of all alleged misconduct. (SOP No. CA-L-S-001)
- Procedures and guidance for recalling data if necessary (SOP No. CA-L-S-001).
- An effective external and internal monitoring system that includes procedures for internal audits (Section 16).

As an American Council of Independent Laboratories (ACIL) member, all TestAmerica laboratories adhere to the following ACIL Code of Ethics:

- Produce results, which are accurate and include QA/QC information that meets client pre-defined Data Quality Objectives (DQOs).
- Present services in a confidential, honest and forthright manner.
- Provide employees with guidelines and an understanding of the ethical and quality standards of our industry.
- Operate our facilities in a manner that protects the environment and the health and safety of employees and the public.
- Obey all pertinent federal, state and local laws and regulations and encourage other members of our industry to do the same.
- Educate clients as the extent and kinds of services available.
- Assert competency only for work for which adequate personnel and equipment are available and for which adequate preparation has been made.
- Promote the status of environmental laboratories, their employees, and the value of services rendered by them.

### **5.3 QUALITY SYSTEM SUPPORTING DOCUMENTATION**

The laboratory's Quality System is communicated through a variety of documents prepared by the laboratory and company management:

- Quality Assurance Manual (QAM) Template
- Quality Assurance Manual – Each laboratory has a lab specific quality assurance manual.
- Corporate SOPs and Policies - Corporate SOPs and Policies are developed for use by all relevant laboratories. They are incorporated into the laboratory's normal SOP distribution, training and tracking system. Corporate SOPs may be general or technical.
- Work Instructions - A subset of procedural steps, tasks or forms associated with an operation of a management system (e.g., checklists, preformatted bench sheets, forms).
- Laboratory SOPs – General and Technical
- Corporate TestAmerica QA/QC Policy Memorandums (Refer to Section 3.4).
- Laboratory QA/QC Policy Memorandums (Refer to Section 3.4).

#### **5.3.1 Order of Precedence**

In the event of a conflict or discrepancy between policies, the order of precedence is as follows:

- TestAmerica QA/QC Policy Memorandum - Corporate
- Laboratory QA/QC Policy Memorandum
- Quality Assurance Manual
- Corporate SOPs and Policies
- Laboratory SOPs and Policies

- Other (Work Instructions (WI), memos, flow charts, etc.)

#### **5.4 QA/QC OBJECTIVES FOR THE MEASUREMENT OF DATA**

Quality Assurance (QA) and Quality Control (QC) are activities undertaken to achieve the goal of producing data that accurately characterize the sites or materials that have been sampled. Quality Assurance is generally understood to be more comprehensive than Quality Control. Quality Assurance can be defined as the integrated system of activities that ensures that a product or service meets defined standards.

Quality Control is generally understood to be limited to the analyses of samples and to be synonymous with the term "*analytical quality control*". QC refers to the routine application of statistically based procedures to evaluate and control the accuracy of results from analytical measurements. The QC program includes procedures for estimating and controlling precision and bias and for determining reporting limits.

Request for Proposals (RFPs) and Quality Assurance Project Plans (QAPP) provide a mechanism for the client and the laboratory to discuss the data quality objectives in order to ensure that analytical services closely correspond to client needs. The client is responsible for developing the QAPP. In order to ensure the ability of the laboratory to meet the Data Quality Objectives (DQOs) specified in the QAPP, clients are advised to allow time for the laboratory to review the QAPP before being finalized. Additionally, the laboratory will provide support to the client for developing the sections of the QAPP that concern laboratory activities.

Historically, laboratories have described their QC objectives in terms of precision, accuracy, representativeness, comparability, completeness, selectivity and sensitivity (PARCCSS).

##### **5.4.1 Precision**

The laboratory objective for precision is to meet the performance for precision demonstrated for the methods on similar samples and to meet data quality objectives of the EPA and/or other regulatory programs. Precision is defined as the degree of reproducibility of measurements under a given set of analytical conditions (exclusive of field sampling variability). Precision is documented on the basis of replicate analysis, usually duplicate or matrix spike (MS) duplicate samples. The calculation of precision is described in Section 25.

##### **5.4.2 Accuracy**

The laboratory objective for accuracy is to meet the performance for accuracy demonstrated for the methods on similar samples and to meet data quality objectives of the EPA and/or other regulatory programs. Accuracy is defined as the degree of bias in a measurement system. Accuracy may be documented through the use of laboratory control samples (LCS) and/or MS. A statement of accuracy is expressed as an interval of acceptance recovery about the mean recovery. The calculation of accuracy is described in Section 25.

#### **5.4.3 Representativeness**

The laboratory objective for representativeness is to provide data which is representative of the sampled medium. Representativeness is defined as the degree to which data represent a characteristic of a population or set of samples and is a measurement of both analytical and field sampling precision. The representativeness of the analytical data is a function of the procedures used in procuring and processing the samples. The representativeness can be documented by the relative percent difference between separately procured, but otherwise identical samples or sample aliquots.

The representativeness of the data from the sampling sites depends on both the sampling procedures and the analytical procedures. The laboratory may provide guidance to the client regarding proper sampling and handling methods in order to assure the integrity of the samples.

#### **5.4.4 Comparability**

The comparability objective is to provide analytical data for which the accuracy, precision, representativeness and reporting limit statistics are similar to these quality indicators generated by other laboratories for similar samples, and data generated by the laboratory over time.

The comparability objective is documented by inter-laboratory studies carried out by regulatory agencies or carried out for specific projects or contracts, by comparison of periodically generated statements of accuracy, precision and reporting limits with those of other laboratories, and by the degree to which approval from the US EPA or other pertinent regulatory agencies is obtained for any procedure for which significant modifications have been made.

#### **5.4.5 Completeness**

The completeness objective for data is 90% (or as specified by a particular project), expressed as the ratio of the valid data to the total data over the course of the project. Data will be considered valid if they are adequate for their intended use. Data usability will be defined in a QAPP, project scope or regulatory requirement. Data validation is the process for reviewing data to determine its usability and completeness. If the completeness objective is not met, actions will be taken internally and with the data user to improve performance. This may take the form of an audit to evaluate the methodology and procedures as possible sources for the difficulty or may result in a recommendation to use a different method.

#### **5.4.6 Selectivity**

Selectivity is defined as: The capability of a test method or instrument to respond to a target substance or constituent in the presence of non-target substances. Target analytes are separated from non-target constituents and subsequently identified/detected through one or more of the following, depending on the analytical method: extractions (separation), digestions (separation), interelement corrections (separation), use of matrix modifiers (separation), specific retention times (separation and identification), confirmations with different columns or detectors (separation and identification), specific wavelengths (identification), specific mass spectra (identification), specific electrodes (separation and identification), etc.

#### **5.4.7 Sensitivity**

Sensitivity refers to the amount of analyte necessary to produce a detector response that can be reliably detected (Method Detection Limit) or quantified (Reporting Limit).

### **5.5 CRITERIA FOR QUALITY INDICATORS**

The laboratory prepares a Reference Data Summary from the LIMS that contains tables that summarize the precision and accuracy acceptability limits for analyses performed at TestAmerica West Sacramento. This summary includes an effective date, is updated each time new limits are generated and is located in the Quality Assurance Department files. A database tracks the effective dates, generation dates, LIMS list number, matrices and archive status of the data utilized to generate the precision and acceptability limits. Unless otherwise noted, limits within these tables are laboratory generated. Some acceptability limits are derived from US EPA methods when they are required. Where US EPA method limits are not required, TestAmerica West Sacramento has developed limits from evaluation of data from similar matrices. Criteria for development of control limits is contained in Section 25.

### **5.6 STATISTICAL QUALITY CONTROL**

Statistically-derived precision and accuracy limits are required by selected methods (such as SW-846) and programs [such as the Ohio Voluntary Action Plan (VAP)]. TestAmerica West Sacramento routinely utilizes statistically-derived limits to evaluate method performance and determine when corrective action is appropriate. Control limits are derived according to laboratory SOP No. QA-003-SAC, "Quality Control Program". The analysts are instructed to use the current limits in the laboratory (dated and approved by the Operations Manager and/or Department Manager and QA Manager) and entered into the Laboratory Information Management System (LIMS). The Quality Assurance department maintains an archive of all limits used within the laboratory. If a method defines the QC limits, the method limits are used.

If a method requires the generation of historical limits, the lab develops such limits from recent data in the QC database of the LIMS following the guidelines described in Section 25. All calculations and limits are documented and dated when approved and effective. On occasion, a client requests contract-specified limits for a specific project.

Surrogate recoveries are determined for a specific time period as defined above. The resulting ranges are entered in LIMS.

Current QC limits are entered and maintained in the LIMS analyte database. As sample results and the related QC are entered into LIMS, the sample QC values are compared with the limits in LIMS to determine if they are within the acceptable range. The analyst then evaluates if the sample needs to be rerun or re-extracted/rerun or if a comment should be added to the report explaining the reason for the QC outlier.

#### **5.6.1 QC Charts**

As the QC limits are calculated, QC charts are generated showing warning and control limits for the purpose of evaluating trends. The QA Manager evaluates these to determine if adjustments need to be made or for corrective actions to methods. All findings are documented and kept on

file. Control charts are generated according to laboratory SOP No. QA-003-SAC, "Quality Control Program".

## **5.7 QUALITY SYSTEM METRICS**

In addition to the QC parameters discussed above, the entire Quality System is evaluated on a monthly basis through the use of specific metrics (refer to Section 17). These metrics are used to drive continuous improvement in the laboratory's Quality System.

## SECTION 6

### DOCUMENT CONTROL (NELAC 5.4.3)

#### 6.1 OVERVIEW

The QA Department is responsible for the control of documents used in the laboratory to ensure that approved, up-to-date documents are in circulation and out-of-date (obsolete) documents are archived or destroyed. The following documents, at a minimum, must be controlled at each laboratory Facility:

- Laboratory Quality Assurance Manual
- Laboratory Standard Operating Procedures (SOP)
- Laboratory Policies
- Work Instructions and Forms
- Corporate Policies and Procedures distributed outside the intranet

The Corporate staff posts Corporate Manuals, SOPs, Policies, Work Instructions, White Papers and Training Materials on the company intranet site. These are collectively termed "Official Documents" and encompass the Policies and Procedures that all facilities are required to employ. These official documents are only considered controlled when they are read on the company intranet site. Printed copies are considered uncontrolled unless the laboratory physically distributes them as controlled documents. A detailed description of the procedure for issuing, authorizing, controlling, distributing, and archiving official documents is found in Corporate SOP No. CW-Q-S-001, Corporate Document Control and Archiving. Distribution at the laboratory is found in the laboratory SOP No. WS-QA-0021, Preparation and Management of Standard Operating Procedures.

The laboratory QA Department also maintains access to various references and document sources integral to the operation of the laboratory. This includes reference methods and regulations. Instrument manuals (hard or electronic copies) are also maintained by the laboratory.

The laboratory maintains control of records for raw analytical data and supporting records such as audit reports and responses, logbooks, standard logs, training files, MDL studies, Proficiency Testing (PT) studies, certifications and related correspondence, and corrective action reports. Raw analytical data consists of bound logbooks, instrument printouts, any other notes, magnetic media, electronic data and final reports. Discussion on records control is described in Section 15.

The maintenance of purchasing data is discussed in Section 9.

The maintenance of sales and marketing contracts is discussed in Section 7.

#### 6.2 DOCUMENT APPROVAL AND ISSUE

The pertinent elements of a control system for each document include a unique name and number, the number of pages of the item, the effective date, revision number and the

laboratory's name. The QA Manager is responsible for the maintenance of the system and maintains the items electronically, in addition to hardcopies in the Quality Assurance Department Office.

Controlled documents are authorized by the QA Department and other management. In order to develop a new document, a manager submits an electronic draft to the QA Department for suggestions and approval before use. Upon approval, QA personnel add the identifying version information to the document and retains the official document on file. The official document is provided as needed to those using it. Controlled documents shall be available at all locations where the operational activity described in the document is performed (may include electronic access). Controlled documents are identified as such and records of their distribution are kept by the QA Department. Document control may be achieved by either electronic or hardcopy distribution.

The QA Department maintains a list of the official versions of controlled documents.

Quality System Policies and Procedures will be reviewed at a minimum of every year and revised as appropriate. Changes to documents occur when a procedural change warrants a revision of the document.

### **6.3 PROCEDURES FOR DOCUMENT CONTROL POLICY**

For changes to the QA Manual, refer to SOP No. WS-QA-0021, Preparation and Management of Standard Operating Procedures. Uncontrolled copies must not be used within the laboratory. Previous revisions and back-up data are stored by the QA department. Electronic copies are stored on the Public server in the QA folder for the applicable revision, and are accessible using the laboratory's Intranet.

For changes to SOPs, refer to SOP No. WS-QA-0021, Preparation and Management of Standard Operating Procedures.

Forms, worksheets, work instructions and information are organized by department in the QA office. There is a table of contents. Electronic versions are kept on a network drive in the QA department; hard copies are kept in QA files. The procedure for the care of these documents is in SOP No. WS-QA-0021, Preparation and Management of Standard Operating Procedures.

### **6.4 OBSOLETE DOCUMENTS**

All invalid or obsolete documents are removed, or otherwise prevented from unintended use. The laboratory has specific procedures as described above to accomplish this. In general, obsolete documents are collected from employees according to distribution lists and are marked obsolete on the cover or destroyed. At least one copy of the obsolete document is archived as described in Section 15.

## SECTION 7

### REVIEW OF WORK REQUEST

#### 7.1 OVERVIEW

TestAmerica West Sacramento has established procedures for the review of work requests and contracts, oral or written. The procedures include evaluation of the laboratory's capability and resources to meet the contract's requirements within the requested time period. All requirements, including the methods to be used, must be adequately defined, documented and understood. For many environmental sampling and analysis programs, testing design is site or program specific and does not necessarily "fit" into a standard laboratory service or product. It is TestAmerica's intent to provide both standard and customized environmental laboratory services to our clients.

A thorough review of technical and QC requirements contained in contracts is performed to ensure project success. The appropriateness of requested methods, and the lab's capability to perform them must be established. Projects, proposals and contracts are reviewed for adequately defined requirements and TestAmerica's capability to meet those requirements. Alternate test methods that are capable of meeting the clients' requirements may be proposed by the lab. A review of the lab's capability to analyze non-routine analytes is also part of this review process.

All projects, proposals and contracts are reviewed for the client's requirements in terms of compound lists, test methodology requested, sensitivity (detection and reporting levels), accuracy, and precision requirements (% Recovery and RPD). The reviewer ensures that the laboratory's test methods are suitable to achieve these regulatory and client requirements and that the laboratory holds the appropriate certifications and approvals to perform the work. The laboratory and any potential subcontract laboratories must be certified, as required, for all proposed tests.

The laboratory must determine if it has the necessary physical, personnel and information resources to meet the contract, and if the personnel have the expertise needed to perform the testing requested. Each proposal is checked for its impact on the capacity of the laboratory's equipment and personnel. As part of the review, the proposed turnaround time will be checked for feasibility.

Electronic or hard copy deliverable requirements are evaluated against the lab's capacity for production of the documentation.

If the laboratory cannot provide all services but intends to subcontract such services, whether to another TestAmerica facility or to an outside firm, this will be documented and discussed with the client prior to contract approval. (Refer to Section 8 for Subcontracting Procedures.)

The laboratory informs the client of the results of the review if it indicates any potential conflict, deficiency, lack of accreditation, or inability of the lab to complete the work satisfactorily. Any discrepancy between the client's requirements and TestAmerica's capability to meet those requirements is resolved in writing before acceptance of the contract. It is necessary that the

contract be acceptable to both the laboratory and the client. Amendments initiated by the client and/or TestAmerica, are documented in writing.

All contracts, QAPPs, Sampling and Analysis Plans (SAPs), contract amendments, and documented communications become part of the project record.

The review process is repeated when there are amendments to the original contract by the client, and the participating personnel are informed of the changes.

## **7.2 REVIEW SEQUENCE AND KEY PERSONNEL**

Appropriate personnel will review the work request at each stage of evaluation.

For routine projects and other simple tasks, a review by the Project Manager (PM) is considered adequate. The PM confirms that the laboratory has all required certifications, and can meet the clients' data quality and reporting requirements. The PM will also get approval by the Laboratory Director to commit to delivery schedules that are shorter than the published standard TATs. The Laboratory Director updates these TATs on a routine basis, and it is the responsibility of CSMs and PMs to review them prior to making commitments for the laboratory.

It is recommended that, where there is a sales person assigned to the account, an attempt should be made to contact that sales person to inform them of the incoming samples.

If the project is an air, drinking water, or hi-res opportunity, a message describing the opportunity will be immediately sent to the appropriate specialty market distribution list.

New opportunities with an estimated value greater than \$100K are passed to the laboratory CSM or BDM, and a message regarding the project details is immediately forwarded to the Large Opportunity Tracking (LOT) distribution list. Specialty market distribution will be included in this notification as appropriate, as well as the associated sales person.

The contract review process is outlined in SOP No. CA-L-P-002, Contract Compliance Policy.

This review encompasses all facets of the operation. The scope of work is distributed to the appropriate personnel, as needed based on scope of contract, to evaluate all of the requirements shown above (not necessarily in the order below.)

- Legal & Contracts Director
- General Manager
- The Customer Service Manager
- The Business Development Manager
- Laboratory and/or Corporate Technical Directors
- Laboratory and/or Corporate Information Technology Managers/Directors
- Regional and/or National Account representatives
- Laboratory and/or Corporate Quality
- Laboratory and/or Corporate Environmental Health and Safety Managers/Directors
- The Laboratory Director reviews the formal laboratory quote and makes final acceptance for their facility.

The National Account Director, Legal Contracts Director, or local account representative then submits the final proposal to the client.

In the event that one of the above personnel is not available to review the contract, his or her back-up will fulfill the review requirements.

The Legal & Contracts Director maintains copies of all signed contracts, as does the local Business Development Manager.

### **7.3 DOCUMENTATION**

Appropriate records are maintained for every contract or work request. All stages of the contract review process are documented and include records of any significant changes. Contract negotiations and finalization is the responsibility of the Business Development Manager. These records are archived by client and project in a restricted network folder accessible to laboratory department managers, project managers, and senior managers.

Records are maintained of pertinent discussions with a client relating to the client's requirements or the results of the work during the period of execution of the contract. Each Laboratory Project Manager keeps a phone log of conversations with the client. In addition, all conversations involving notification of important information, or actions directed by the client are documented with a follow up e-mail and archived in the contracts folder or the SDG documentation and case narrative. Instances include change in scope, alterations to the requests listed on a chain of custody, directions to proceed in the event of a non-conformance, and any other conversation that changes the direction of a COC or contract.

#### **7.3.1 Project-Specific Quality Planning**

Communication of contract specific technical and QC criteria is an essential activity in ensuring the success of site specific testing programs. To achieve this goal, TestAmerica West Sacramento assigns a PM to each client that is the first point of contact for the client. It is the PM's responsibility to ensure that project specific technical and QC requirements are effectively evaluated and communicated to the laboratory personnel before and during the project. QA department involvement may be needed to assist in the evaluation of custom QC requirements.

PM's are the direct client contact and they ensure resources are available to meet project requirements. They coordinate opportunities and forecast incoming work, allowing the laboratory management team to ensure available resources are sufficient to perform work for the client's project. Project management is positioned between the client and laboratory resources.

Prior to work on a new program, the Laboratory Project Managers record project details and requirements via the Quality Assurance Summary (QAS.) Each laboratory backlog automatically incorporates the pertinent project specific information into a single resource for the bench level chemist. In addition, Project Managers may also choose to lead a project kick-off meeting and discuss QAS items in detail, as well as key events and challenges. The Laboratory Department Managers are responsible for guiding their team's compliance, and use the Project Managers and QA Manager to interpret requirements and resolve conflicts.

During the project, any change that may occur within an active project is agreed upon between the client and the laboratory. These changes (e.g., use of a non-standard method or modification of a method) and approvals must be documented prior to implementation. Documentation pertains to any document, e.g., letter, e-mail, variance, contract addendum, which has been signed (or acknowledged via e-mail) by both parties.

Such changes are updated to the QAS and introduced to the managers at these meetings. The laboratory staff is then introduced to the modified requirements via the PM or the individual laboratory Department Manager. After the modification is implemented into the laboratory process, documentation of the modification is made in the case narrative of the data report(s).

TestAmerica strongly encourages client visits to the laboratory and for formal/informal information sharing session with employees in order to effectively communicate ongoing client needs as well as project specific details for customized testing programs.

## SECTION 8

### SUBCONTRACTING OF TESTS (NELAC 5.4.5)

#### 8.1 OVERVIEW

For the purpose of this quality manual, the phrase subcontract laboratory refers to a laboratory external to the corporate network. The phrase “work sharing” refers to internal transfers of samples between company laboratories. The term outsourcing refers to the act of subcontracting tests.

When contracting with our clients, the laboratory makes commitments regarding the services to be performed and the data quality for the results to be generated. When we must outsource testing for our clients because project scope, changes in laboratory capabilities, capacity or unforeseen circumstances, we must be assured that the subcontractors or work sharing laboratories understand the requirements and will meet the same commitments we have made to the client. Refer to the SOP on Subcontracting Procedures (CA-L-S-002) and the Work Sharing Process SOP (CA-C-S-001).

When outsourcing analytical services, the laboratory will assure, to the extent necessary, that the subcontract or work sharing laboratory maintains a program consistent with the requirements of this document, the requirements specified in NELAC/ISO 17025 and/or the client’s Quality Assurance Project Plan (QAPP). All QC guidelines specific to the client’s analytical program are transmitted to the subcontractor and agreed upon before sending the samples to the subcontract facility. Additionally, work requiring accreditation will be placed with an appropriately accredited laboratory. The laboratory performing the subcontracted work will be identified in the final report, as will non-NELAC accredited work where required.

For DOD projects the subcontractor laboratories used must have an established and documented laboratory quality system that complies with DoD QSM requirements. The subcontractor laboratories are evaluated following the procedures outlined below and as seen in Figure 8-1. The subcontractor laboratory must receive project-specific approval from the DoD client before any samples are analyzed.

The QSM has 5 specific requirements for subcontracting:

1. Subcontractor laboratories must have an established laboratory quality system that complies with the QSM.
2. Subcontractor laboratories must be approved by the specific DoD Component laboratory approval process.
3. Subcontractor laboratories must demonstrate the ability to generate acceptable results from the analysis of PT samples, subject to availability, using each applicable method, in the specified matrix, and provide appropriate documentation to the DoD client.
4. Subcontractor laboratories must receive project-specific approval from the DoD client before any samples are analyzed.
5. Subcontractor laboratories are subject to project-specific, on-site assessments by the DoD client or their designated representatives.

Project Managers (PMs), Customer Service Managers (CSM), or Regional Account Executives (RAE) for the Export Lab are responsible for obtaining client approval prior to outsourcing any samples. The laboratory will advise the client of a subcontract or work sharing arrangement in writing and when possible approval from the client shall be retained in the project folder.

**Note:** In addition to the client, some regulating agencies, such as the US Army Corps of Engineers and the USDA, require notification prior to placing such work. Documentation of approval is stored electronically in the QBIS folder on the “world” share on the laboratory’s server.

## **8.2 QUALIFYING AND MONITORING SUBCONTRACTORS**

Whenever a PM or Customer Service Manager (CSM) becomes aware of a client requirement or laboratory need where samples must be outsourced to another laboratory, the other laboratory(s) shall be selected based on the following:

- The first priority is to attempt to place the work in a qualified network laboratory;
- Firms specified by the client for the task (Documentation that a subcontractor was designated by the client must be maintained with the project file. This documentation can be as simple as placing a copy of an e-mail from the client in the project folder);
- Firms listed as pre-qualified and currently under a subcontract with the company (in JD Edwards): A listing of all approved subcontracting laboratories and supporting documentation is available on the TestAmerica intranet site. Verify necessary accreditation for the requested tests prior to sending samples.
- Firms identified in accordance with the company’s Small Business Subcontracting program as small, women-owned, veteran-owned and/or minority-owned businesses;
- NELAC or A2LA accredited laboratories.
- In addition, the firm must hold the appropriate certification to perform the work required.

All intra-company laboratories are pre-qualified for work sharing provided they hold the appropriate accreditations, can adhere to the project/program requirements, and the client approved sending samples to that laboratory. The client must provide acknowledgement that the samples can be sent to that facility (an e-mail is sufficient documentation or if acknowledgement is verbal, the date, time, and name of person providing acknowledgement must be documented). The originating laboratory is responsible for communicating all technical, quality, and deliverable requirements as well as other contract needs. Refer to SOP No. CA-C-S-001, Work Sharing Process.

When the potential sub-contract laboratory has not been previously approved, PMs or CSMs may nominate a laboratory as a subcontractor based on need. The decision to nominate a laboratory must be approved by the Laboratory Director. The Laboratory Director requests that the QA Manager begin the process of approving the subcontract laboratory. The client must provide acknowledgement that the samples can be sent to that facility (an e-mail is sufficient documentation or if acknowledgement is verbal, the date, time, and name of person providing acknowledgement must be documented).

**8.2.1** The QA Manager must ensure that the Subcontracting Approval Form (Figure 8-1)

has been completed and have supporting documentation on file prior to initiation of any work. A letter or e-mail is sent to the lab requesting the following information:

- 8.2.1.1** If a lab is NELAC or A2LA accredited,
  - 8.2.1.1.1** Copy of necessary certifications verifying that the required approvals are current. Ensure that all needed analytes are included; some may not be accredit-able (if so, document). Certificate and scope of International Standard accreditation are required, when applicable.
  - 8.2.1.1.2** Insurance Certificate. This is required by TestAmerica's Chief Financial Officer
  - 8.2.1.1.3** USDA soil permit if available\*\*
- 8.2.1.2** For Laboratories accredited by other agencies with an auditing program:
  - 8.2.1.2.1** Copy of necessary certifications verifying that the required approvals are current. Ensure that all needed analytes are included; some may not be accredit-able (if so, document). Certificate and scope of International Standard accreditation are required, when applicable.
  - 8.2.1.2.2** Insurance Certificate. This is required by TestAmerica's Chief Financial Officer
  - 8.2.1.2.3** USDA soil permit if available\*\*
  - 8.2.1.2.4** Description of Ethics and Data Integrity Plan.
  - 8.2.1.2.5** The most recent 2 sets of full proficiency testing (PT) results relevant to the analyses of interest and any associated corrective action.
  - 8.2.1.2.6** State Audit with Corrective Action Response
  - 8.2.1.2.7** Example final report to confirm format is compliant and provides the necessary information. Minimally, it must be determined that Batch QC results are included in the laboratory reports and data is appropriately qualified.
  - 8.2.1.2.8** A copy of raw data associated with the first project is requested for internal review. The raw data is reviewed by the QA Manager and the PM to ensure that the results meet the client's needs. If the QA manager is unfamiliar with the analysis being performed, notify Corporate QA for guidance on the review (it may need to be sent elsewhere for evaluation). This requirement can be skipped if an on-site visit of the laboratory is planned. (This requirement is effective as of the effective date of this section. Laboratories worked with previously [minimum of 6 months] are grandfathered in.)
  - 8.2.1.2.9** DoD work includes additional requirements as described in Section 8.1 above.
- 8.2.1.3** For laboratories performing tests that are unaccredited or accredited by an agency without an audit program:

- 8.2.1.3.1** A copy of their Quality Assurance Manual (controlled if possible). Ensure data quality limits for relevant methods are acceptable and that training procedures are adequate.
  - 8.2.1.3.2** Copy of necessary certifications (if available) verifying that the required approvals are current. Ensure that all needed analytes are included; some may not be accredit-able (if so, document). Certificate and scope of International Standard accreditation are required, when applicable.
  - 8.2.1.3.3** Insurance Certificate. This is required by TestAmerica's Chief Financial Officer.
  - 8.2.1.3.4** USDA soil permit if available\*\*
  - 8.2.1.3.5** Evidence of a current SOP per method. A copy of the first page and signature page of the SOP is acceptable. A table of contents including effective dates may also be acceptable. The SOP can be examined if an on-site audit is performed.
  - 8.2.1.3.6** Description of Ethics and Data Integrity Plan.
  - 8.2.1.3.7** The most recent 2 sets of full proficiency testing (PT) results relevant to the analyses of interest and any associated corrective action.
  - 8.2.1.3.8** Example final report to confirm format is compliant and provides the necessary information. Minimally, it must be determined that Batch QC results are included in the laboratory reports and data is appropriately qualified.
  - 8.2.1.3.9** Statement of Qualification (SOQ) or summary list of Technical Staff and Qualifications – position, education and years of experience.
  - 8.2.1.3.10** DoD work includes additional requirements as described in Section 8.1 above.
  - 8.2.1.3.11** A copy of raw data associated with the first project is requested for internal review. The raw data is reviewed by the QA Manager and the PM to ensure that the results meet the client's needs. If the QA manager is unfamiliar with the analysis being performed, notify Corporate QA for guidance on the review (it may need to be sent elsewhere for evaluation). This requirement can be skipped if an on-site visit of the laboratory is planned. (This requirement is effective as of the effective date of this section. Laboratories worked with previously [minimum of 6 months] are grandfathered in.)
- 8.2.2** Once the information is received by the QA Manager, it is evaluated for acceptability and forwarded to Corporate Contracts for formal contracting with the laboratory. They will add the lab to the approved list on the intranet site along with the associate documentation and notify the finance group for JD Edwards.

\*\*USDA permit is required if soils less than three feet deep from New York, North Carolina, South Carolina, Georgia, Florida, Tennessee, Alabama, Mississippi, Louisiana, Arkansas, Texas, Oklahoma, New Mexico, Arizona, California, Hawaii, or outside the continental U. S. are

to be analyzed. These samples require special shipping measures; check with the EHS Department. It may be necessary to heat-treat the samples before shipping if the subcontract laboratory does not have a USDA permit; however, some analytes/tests may be irrelevant after heat treatment.

**8.2.3** The client will assume responsibility for the quality of the data generated from the use of a subcontractor they have requested the lab to use. The qualified subcontractors on the intranet site are known to meet minimal standards. The company does not certify laboratories. The subcontractor is on our approved list and can only be recommended to the extent that we would use them.

**8.2.4** The status and performance of qualified subcontractors will be monitored periodically by the Corporate Contract Department. Any problems identified will be brought to Corporate QA attention.

- Complaints shall be investigated. Documentation of the complaint, investigation and corrective action will be maintained in the subcontractor's file on the intranet site. Complaints must be posted using the Vendor Performance Report (Form No. CW-F-WI-009).
- Information must be updated on the intranet when new information is received from the subcontracted laboratories.
- Subcontractors in good standing will be retained on the intranet listing. The QA Manager will notify all network laboratories and Corporate QA and Corporate Contracts if any laboratory requires removal from the intranet site. This notification will be posted on the intranet site and e-mailed to all Lab Directors/Managers, QA Managers and Sales Directors.

### **8.3 OVERSIGHT AND REPORTING**

The PM must request that the selected subcontractor be presented with a subcontract, if one is not already executed between the laboratory and the subcontractor. The subcontract must include terms which flow down the requirements of our clients, either in the subcontract itself or through the mechanism of work orders relating to individual projects. A standard subcontract and the Lab Subcontractor Vendor Package (posted on the intranet) can be used to accomplish this, and the Legal & Contracts Director can tailor the document or assist with negotiations, if needed. The PM (or CSM) responsible for the project must advise and obtain client consent to the subcontract as appropriate, and provide the scope of work to ensure that the proper requirements are made a part of the subcontract and are made known to the subcontractor.

Prior to sending samples to the subcontracted laboratory, the PM confirms their certification status to determine if it's current and scope-inclusive. The information is documented in the QBIS directory in the project folder, and is retained in the Quality Assurance office. For network laboratories, certifications can be viewed on the company website.

The Sample Control department is responsible for ensuring compliance with QA requirements and applicable shipping regulations when shipping samples to a subcontracted laboratory.

All subcontracted samples must be accompanied by a Chain of Custody (COC). A copy of the original COC sent by the client must be included with all samples subbed within the network.

The PM will communicate with the subcontracted laboratory to monitor the status of the analyses, facilitate successful execution of the work and ensure the timeliness and completeness of the analytical report.

Non-NELAC accredited work must be identified in the subcontractor's report as appropriate. If NELAC accreditation is not required, the report does not need to include this information.

Reports submitted from subcontractor laboratories are not altered and are included in their original form in the final project report. This clearly identifies the data as being produced by a subcontractor facility. Results submitted by a network work-sharing laboratory on the same LIMS will be designated in the case narrative.

**Note:** The results submitted by a network work sharing laboratory may be transferred electronically and the results reported by the network work sharing lab are identified on the final report. The report must explicitly indicate which lab produced the data for which methods and samples. The final report must include a copy of the completed COC for all work sharing reports.

#### **8.4 CONTINGENCY PLANNING**

The Laboratory Director may waive the full qualification of a subcontractor process temporarily to meet emergency needs. In the event this provision is utilized, Corporate QA must be informed, and the QA Manager will be required to verify adequacy of proficiency scores and certifications. The laboratory must also request a copy of the raw data to support the analytical results for the first project submitted to the subcontract laboratory unless the laboratory has NELAC accreditation. The raw data is reviewed by the QA Manager and the PM to ensure that the results meet the client's needs. The QA Manager will request full documentation and qualify the subcontractor under the provisions above. The approval process should be completed within 30 calendar days of subcontracting.

**Figure 8-1.  
Example - Subcontracting Laboratory Approval Form (Initial / Renewal)**

**SUBCONTRACTING LABORATORY APPROVAL**

*Reference: Section 8 – Quality Assurance Manual*

---

Date: \_\_\_\_\_  
Laboratory: \_\_\_\_\_  
Address: \_\_\_\_\_  
Contact and e-mail address: \_\_\_\_\_  
Phone: Direct \_\_\_\_\_ Fax \_\_\_\_\_

---

Requested Item <sup>3</sup>	Date Received	Reviewed/ Accepted	Date
1. Copy of State Certification <sup>1</sup>			
2. Insurance Certificate			
3. USDA Soil Permit			
4. Description of Ethics Program <sup>3</sup>			
5. QA Manual <sup>3</sup>			
6. Most Recent (and relevant) 2 Sets of WP/WS Reports with Corrective Action Response <sup>1,3</sup>			
7. State Audit with Corrective Action Response (or NELAC or A2LA Audit) <sup>3</sup>			
8. Sample Report <sup>3</sup>			
9. SOQ or Summary list of Technical Staff and Qualifications <sup>3</sup>			
10. SOPs for Methods to Be Loadshifted <sup>2,3</sup>			
11. For DoD Work: Statement that Lab quality system complies with QSM.			
12. For DoD Work: Approved by specific DoD Component laboratory approval process.			

1 - Required when emergency procedures are implemented.  
2 - Some labs may not submit copies due to internal policies. In these cases, a copy of the first page and signature page of the SOP is acceptable. This requirement may also be fulfilled by supplying a table of SOPs with effective dates.  
3 - If the laboratory has NELAC accreditation, Item #s 4 through 10 are not required.

On Site Audit Planned: YES NO If yes, Date Completed: \_\_\_\_\_ By Whom: \_\_\_\_\_

Comments:  
\_\_\_\_\_

Lab Acceptable for Subcontracting Work: YES NO Limitations: \_\_\_\_\_

QA Manager (Signature): \_\_\_\_\_ Date: \_\_\_\_\_  
(Printed Name)

Forwarded to Contract Coordinator by: \_\_\_\_\_ Date: \_\_\_\_\_

## SECTION 9

### PURCHASING SERVICES AND SUPPLIES (NELAC 5.4.6)

#### 9.1 OVERVIEW

Evaluation and selection of suppliers and vendors is performed, in part, on the basis of the quality of their products, their ability to meet the demand for their products on a continuous and short term basis, the overall quality of their services, their past history, and competitive pricing. This is achieved through evaluation of objective evidence of quality furnished by the supplier, which can include certificates of analysis, recommendations, and proof of historical compliance with similar programs for other clients. To ensure that quality critical consumables and equipment conform to specified requirements, all purchases from specific vendors are approved by a member of the supervisory or management staff.

Capital expenditures are made in accordance with the Controlled Purchases Procedure, CW-F-S-004. Only one quote is required where the item being purchased is a sole source product, Examples of sole source capital expenditures are laboratory test equipment, client specified purchases and building leases. A minimum of two quotes is required where the opportunity exists to source from more than one vendor. All documentation related to the purchase of capital items will be maintained in the individual CapEx files located in Corporate Purchasing. Data will be held in accordance with the record retention policy.

TestAmerica will enter into formal contracts with vendors when it is advantageous to do so. Contracts will be signed in accordance with the Authorization Matrix Policy, CW-F-P-002. Examples of items that are purchased through vendor contracts are laboratory instruments, consumables, copiers and office supplies. Request for Proposals (RFP's) will be issued where more information is required from the potential vendors than just price. RFP's allow TestAmerica to determine if a vendor is capable of meeting requirements such as supplying all of the TestAmerica facilities, meeting required quality standards and adhering to necessary ethical and environmental standards. The RFP process also allows potential vendors to outline any additional capabilities they may offer.

Non-capital expenditure items are purchased through the requisition and approval process in JD Edwards or through other TestAmerica authorized methods (approved web-sites, purchasing cards). Labs have the ability to select from the approved vendors in JD Edwards.

#### 9.2 GLASSWARE

Glassware used for volumetric measurements must be Class A or verified for accuracy according to laboratory procedure. Pyrex (or equivalent) glass should be used where possible. For safety purposes, thick-wall glassware should be used where available.

#### 9.3 REAGENTS, STANDARDS & SUPPLIES

Chemical reagents, solvents, glassware, and general supplies are ordered as needed to maintain sufficient quantities on hand. Purchasing guidelines for equipment and reagents must meet with the requirements of the specific method and testing procedures for which they are

being purchased. Solvents and acids are pre-tested in accordance with Corporate SOP on Solvent & Acid Lot Testing & Approval, SOP No. CA-Q-S-001.

### **9.3.1 Purchasing**

The nature of the analytical laboratory demands that all material used in any of the procedures is of a known quality. The wide variety of materials and reagents available makes it advisable to specify recommendations for the name, brand, and grade of materials to be used in any determination. This information is contained in the method SOP.

Only personnel trained in the ordering program JDE may place orders using the program. All relevant information, including quantity, must be entered. Only approved vendors may be used. A vendor must be approved by corporate to be on the approved vendor list in JDE. The Laboratory Director or designee approves all orders placed in JDE.

### **9.3.2 Receiving**

It is the responsibility of the facilities manager to receive the shipment. It is the responsibility of the analyst who ordered the materials to date the material when received. Once the ordered reagents or materials are received, the analyst compares the information on the label or packaging to the original order to ensure that the purchase meets the quality level specified. Material Safety Data Sheets (MSDSs) are kept in the Hazardous Materials Technician's Office and online through the Company's intranet website. Anyone may review these for relevant information on the safe handling and emergency precautions of on-site chemicals.

### **9.3.3 Specifications**

There are many different grades of analytical reagents available to the analyst. All methods in use in the laboratory specify the grade of reagent that must be used in the procedure. If the quality of the reagent is not specified, it may be assumed that it is not significant in that procedure and, therefore, any grade reagent may be used. It is the responsibility of the analyst to check the procedure carefully for the suitability of grade of reagent.

Chemicals must not be used past the manufacturer's expiration date and must not be used past the expiration time noted in a method SOP. If dates are not provided, the laboratory may contact the manufacturer to determine an expiration date.

The laboratory assumes a five year expiration date on inorganic dry chemicals unless noted otherwise by the manufacturer or by the reference source method.

Wherever possible, standards must be traceable to national or international standards of measurement or to national or international reference materials. Records to that effect are available to the user.

Compressed gases in use are checked for pressure and secure positioning every other day. The minimum total pressure must be 250 psig for the automatic bank of gas tanks before the system switches to the next bank of tanks. No individual compressed gas tanks are used at the instrument benches at TestAmerica West Sacramento. The quality of the gases must meet

method or manufacturer specification or be of a grade that does not cause any analytical interference.

Water used in the preparation of standards or reagents must have a conductivity of less than 1.0 umho/cm (or resistivity of greater than 1.0 megaohm-cm) at 25°C. The conductivity is checked and recorded daily. If the water's conductivity is less than the specified limit, the Operations Manager must be notified immediately in order to notify all departments, decide on cessation (based on intended use) of activities, and make arrangements for correction.

The laboratory may purchase reagent grade (or other similar quality) for use in the laboratory. This water must be certified "clean" by the supplier for all target analytes or otherwise verified by the laboratory prior to use. This verification is documented.

Standard lots are verified before first time use if the laboratory switches manufacturers or has historically had a problem with the type of standard. See laboratory SOP No. WS-QA-0017, "Standards and Reagent Preparation and Quality Control Check Procedures", for standard QC procedures.

Purchased VOA vials must be certified clean and the certificates must be maintained. If uncertified VOA vials are purchased, all lots must be verified clean prior to use. This verification must be maintained.

#### **9.3.4      Storage**

Reagent and chemical storage is important from the aspects of both integrity and safety. Light-sensitive reagents may be stored in brown-glass containers. Table 9-1 details specific storage instructions for reagents and chemicals. Section 22 discusses conditions for standard storage.

### **9.4            PURCHASE OF EQUIPMENT/INSTRUMENTS/SOFTWARE**

When a new piece of equipment is needed, either for additional capacity or for replacing inoperable equipment, the analyst or supervisor makes a supply request to the Technical Director and/or the Laboratory Director. If they agree with the request the procedures outlined in Policy No. CA-T-P-001, Qualified Products List, are followed. A decision is made as to which piece of equipment can best satisfy the requirements. The appropriate written requests are completed and purchasing places the order.

Upon receipt of a new or used piece of equipment, it is given a short name, such as HP-20, and added to the equipment list described in Section 21 that is maintained by the QA Department. IT must also be notified so that the equipment can be linked to have data back-ups performed. Its capability is assessed to determine if it is adequate or not for the specific application. For instruments, a calibration curve is generated, followed by MDLs, Demonstration of Capabilities (DOCs), and other relevant criteria (see Section 20). For software, its operation must be deemed reliable and evidence of instrument verification must be retained by the IT Department or QA Department as specified in the laboratory's procedure for software verification. Software certificates supplied by the vendors are filed with the LIMS Administrator. The manufacturer's operation manual is retained at the bench.

## **9.5 SERVICES**

Service to analytical instruments (except analytical balances) is performed on an as needed basis. Routine preventative maintenance is discussed in Section 21. The need for service is determined by analysts and/or Department Managers. The service providers that perform the services are approved by the Department Managers/Technical Director.

## **9.6 SUPPLIERS**

TestAmerica selects vendors through a competitive proposal / bid process, strategic business alliances or negotiated vendor partnerships (contracts). The level of control used in the selection process is dependent on the anticipated spend and the potential impact on TestAmerica business. Vendors that provide test and measuring equipment, solvents, standards, certified containers, instrument related service contracts or subcontract laboratory services shall be subject to more rigorous controls than vendors that provide off-the-shelf items of defined quality that meet the end use requirements. The JD Edwards purchasing system includes all suppliers /vendors that have been approved for use.

Evaluation of suppliers is accomplished by ensuring the supplier ships the product or material ordered and that the material is of the appropriate quality. This is documented by signing off on packing slips or other supply receipt documents. The purchasing documents contain the data that adequately describe the services and supplies ordered.

Any issues of vendor performance are to be reported immediately by the laboratory staff to the Corporate Purchasing Group by completing a Vendor Performance Report (CW-F-WI-009).

The Corporate Purchasing Group will work through the appropriate channels to gather the information required to clearly identify the problem and will contact the vendor to report the problem and to make any necessary arrangements for exchange, return authorization, credit, etc.

As deemed appropriate, the Vendor Performance Reports will be summarized and reviewed to determine corrective action necessary, or service improvements required by vendors

The laboratory has access to a listing of all approved suppliers of critical consumables, supplies and services. This information is provided through the JD Edwards purchasing system.

### **9.6.1 New Vendor Procedure**

TestAmerica employees who wish to request the addition of a new vendor must complete a J.D. Edwards Vendor Add Request Form (CW-F-WI-007 – refer to Figure 9-1).

New vendors are evaluated based upon criteria appropriate to the products or services provided as well as their ability to provide those products and services at a competitive cost. Vendors are also evaluated to determine if there are ethical reasons or potential conflicts of interest with TestAmerica employees that would make it prohibitive to do business with them as well as their financial stability. The QA Department and/or the Technology Director are consulted with vendor and product selection that have an impact on quality.

**Table 9-1.**  
**Storage of Reagents and Chemicals**

<b>Chemical</b>	<b>Storage Requirements</b>
Concentrated Acids and Bases	Stored in the original containers at room temperature. All organic acids must be stored separately from inorganic acids. Acids should not be stored with bases.
Bulk Dry Chemicals	Stored in the original containers at room temperature. All organic acids must be stored separately from inorganic acids. Acids should not be stored with bases.
Working Solutions containing Organic Compounds	Stored as per method recommendation/ requirement. They are generally stored refrigerated at $4^{\circ}\text{C} \pm 2^{\circ}\text{C}$ .
Working Solutions containing only Inorganics	Stored at room temperature; refrigeration is optional.
Flammable Solvents	Stored in solvent cabinets at room temperature.
Non-Flammable Solvents	Stored separately from the flammable solvents in cabinets at room temperature.

**Figure 9-1**  
**Example – JD Edwards Vendor Add Request Form**



JD Edwards Vendor Add Request Form

Vendor name:	Lab location <u>and</u> individual making request:
Vendor address (remit to):	Vendor phone:
Vendor address (remit to):	Vendor fax:
Contact name:	Product / service provided:

**Reason for Vendor Addition: Check all reasons that apply**

<input type="checkbox"/> Cost Reduction	Estimated Annual Savings \$
<input type="checkbox"/> Replace Current Vendor	Reason?
	Vendor being Replaced?
<input type="checkbox"/> New Product / Service	Describe:
<input type="checkbox"/> ISO Approved (Required for Aerotech / P&K only)	

**Small Business:**

Does this vendor help us to meet our small business objectives: \_\_\_\_\_  
 If yes, which category: \_\_\_\_\_

**Personal and Ethical Considerations:**

Is there any personal conflict of interest with a TestAmerica employee and the vendor listed above? \_\_\_\_\_  
 Have ethical considerations been taken into account in your evaluation of this vendor? \_\_\_\_\_  
 \_\_\_\_\_

**Can this product be sourced from another TestAmerica facility?** \_\_\_\_\_

Please complete form and email to [NCPurchasing@testamericainc.com](mailto:NCPurchasing@testamericainc.com) or fax to (330) 966-9275.

I approve the addition of this vendor:

\_\_\_\_\_  
 Purchasing Manager - Patrick Eckman

\_\_\_\_\_  
 Corporate Controller - Leslie Bowers

Form No. CW-F-WI-007

## **SECTION 10**

### **SERVICE TO THE CLIENT (NELAC 5.4.7)**

#### **10.1 OVERVIEW**

TestAmerica West Sacramento cooperates with clients and their representatives to monitor the laboratory's performance in relation to work performed for the client. It is the laboratory's goal to meet all client requirements in addition to statutory and regulatory requirements discussed in Section 5. The laboratory has procedures to ensure confidentiality to clients (Section 16 and 26).

**Note:** ISO 17025/NELAC 2003 states that a laboratory "shall afford clients or their representatives cooperation to clarify the client's request". This topic is discussed in Section 7.

#### **10.2 SPECIAL SERVICES**

The laboratory's standard procedures for reporting data are described in Section 26. When requested the following special services are provided:

- The laboratory will provide the client or the client's representative reasonable access to the relevant areas of the laboratory for the witnessing of tests performed for the client.
- The laboratory will work with client-specified third party data validators as specified in the client's contract.
- The laboratory will provide the client with all requested information pertaining to the analysis of their samples. An additional charge may apply for additional data/information that was not requested prior to the time of sample analysis or previously agreed upon.

#### **10.3 CLIENT COMMUNICATION**

Project managers are an important communication link to the clients. The lab shall inform its clients of any delays in project completion as well as any non-conformances in either sample receipt (refer to Section 24) or sample analysis. Project management will maintain ongoing client communication throughout the entire client project.

Any number of senior staff or technical experts are available to discuss any technical questions or concerns that the client may have.

#### **10.4 REPORTING**

The laboratory will work with the client to produce any special communication reports required by the contract.

**10.5      CLIENT SURVEYS**

The laboratory assesses both positive and negative client feedback. The results are used to improve overall laboratory quality and client service.

TestAmerica's Sales and Marketing teams periodically develops lab and client specific surveys to assess client satisfaction.

## **SECTION 11**

### **COMPLAINTS (NELAC 5.4.8)**

#### **11.1 OVERVIEW**

TestAmerica West Sacramento believes that effective client complaint handling processes have important business and strategic value. Listening to and documenting client concerns captures 'client knowledge' that helps to continually improve processes and improving client satisfaction. An effective client complaint handling process also provides assurance to the data user that the laboratory will stand behind its data, service obligations and products.

A client complaint is any expression of dissatisfaction with any aspect of our business services, communications, responsiveness, data, reports, invoicing and other functions expressed by any party, whether received verbally or in written form. Client inquiries, complaints or noted discrepancies are documented, communicated to management, and addressed promptly and thoroughly.

The laboratory has procedures for dealing with both external and internal complaints.

The nature of the complaint is identified, documented and investigated, and an appropriate action is determined and taken. In cases where a client complaint indicates that an established policy or procedure was not followed, the QA Department must evaluate whether a special audit must be conducted to assist in resolving the issue. A written confirmation or letter to the client, outlining the issue and response taken is recommended as part of the overall action taken.

The process of complaint resolution and documentation utilizes the procedures outlined in Section 13 (Corrective Actions) and is documented following laboratory Policy No. WS-PQA-013, "Procedures to Address Customer Complaint". It is the laboratory's goal to provide a satisfactory resolution to complaints in a timely and professional manner.

#### **11.2 EXTERNAL COMPLAINTS**

An employee that receives a complaint initiates the complaint resolution process and the documentation of the complaint.

Complaints fall into two categories: correctable and non-correctable. An example of a correctable complaint would be one where a report re-issue would resolve the complaint. An example of a non-correctable complaint would be one where a client complains that their data was repeatedly late. Non-correctable complaints should be reviewed for preventive action measures to reduce the likelihood of future occurrence and mitigation of client impact.

The general steps in the complaint handling process are:

- Receiving Complaints
- Complaint Investigation and Service Recovery
- Process Improvement

The laboratory shall inform the initiator of the complaint of the results of the investigation and the corrective action taken, if any.

### **11.3 INTERNAL COMPLAINTS**

Internal complaints include, but are not limited to: errors and non-conformances, training issues, internal audit findings, and deviations from methods. Corrective actions may be initiated by any staff member who observes a nonconformance and shall follow the procedures outlined in Section 13. In addition, Corporate management, Sales and Marketing and Information Technology (IT) may initiate a complaint by contacting the laboratory or through the corrective action system described in Section 13.

### **11.4 MANAGEMENT REVIEW**

The number and nature of client complaints is reported by the QA Manager to the laboratory and QA Director in the QA Monthly report. Monitoring and addressing the overall level and nature of client complaints and the effectiveness of the solutions is part of the Annual Management Review (Section 17)

## SECTION 12

### CONTROL OF NON-CONFORMING WORK (NELAC 5.4.9)

#### 12.1 OVERVIEW

When data discrepancies are discovered or deviations and departures from laboratory standard procedures, policies and/or client requests have occurred, corrective action is taken immediately. First, the laboratory evaluates the significance of the nonconforming work. Then, a corrective action plan is initiated based on the outcome of the evaluation. If it is determined that the nonconforming work is an isolated incident, the plan could be as simple as adding a qualifier to the final results and/or making a notation in the case narrative. If it is determined that the nonconforming work is a systematic or improper practices issue, the corrective action plan could include a more in depth investigation and a possible suspension of an analytical method. In all cases, the actions taken are documented using the laboratory's corrective action system (refer to Section 13).

Due to the frequently unique nature of environmental samples, sometimes departures from documented policies and procedures are needed. When an analyst encounters such a situation, the problem is presented to the Department Manager for advice. The Department Manager may elect to discuss it with the Operations Manager or QA Manager or have a representative contact the client to decide on a logical course of action. Once an approach is agreed upon, the analyst documents it using the laboratories corrective action system described in Section 13. This information can then be supplied to the client in the form of a footnote or a case narrative with the report.

Project Management may encounter situations where a client may request that a special procedure be applied to a sample that is not standard lab practice. Based on a technical evaluation, the lab may accept or opt to reject the request based on technical or ethical merit. An example might be the need to report a compound that the lab does not normally report. The lab would not have validated the method for this compound following the procedures in Section 20. The client may request that the compound be reported based only on the calibration. Such a request would need to be approved by the Laboratory Director and QA Manager, documented and included in the project folder. Deviations **must** also be noted on the final report with a statement that the compound is not reported in compliance with NELAC (or the analytical method) requirements and the reason. Data being reported to a non-NELAC state would need to note the change made to how the method is normally run.

#### 12.2 RESPONSIBILITIES AND AUTHORITIES

SOP No. CA-L-S-001, Internal Investigation of Potential Data Discrepancies and Determination for Data Recall, outlines the general procedures for the reporting and investigation of data discrepancies and alleged incidents of misconduct or violations of the company's data integrity policies as well as the policies and procedures related to the determination of the potential need to recall data.

Under certain circumstances the Laboratory Director, the Operations Manager, or the QA Manager, or their designees may exceptionally authorize departures from documented

procedures or policies. The departures may be a result of procedural changes due to the nature of the sample; a one-time procedure for a client; QC failures with insufficient sample to reanalyze, etc. In most cases, the client will be informed of the departure prior to the reporting of the data. Any departures must be well documented using the laboratory's corrective action procedures described in Section 13. This information may also need to be documented in logbooks and/or data review checklists as appropriate. Any impacted data must be referenced in a case narrative and/or flagged with an appropriate data qualifier.

Any misrepresentation or possible misrepresentation of analytical data discovered by any laboratory staff member must be reported to facility senior laboratory management within 24-hours. The Senior Management staff is comprised of the Laboratory Director, the QA Manager, the Air Toxics Technical Director, the Operations Manager, the Manager of Project Management, and the Business Development Manager. The reporting of issues involving alleged violations of the company's Data Integrity or Manual Integration procedures must be conveyed to an Ethics and Compliance Officer (ECO) and Quality Director within 24 hours.

Whether an inaccurate result was reported due to calculation or quantitation errors, data entry errors, improper practices, or failure to follow SOPs, the data must be evaluated to determine the possible effect.

The Laboratory Director, QA Manager, ECOs, COOs – East and West, General Managers and the Quality Directors – East and West have the authority and responsibility to halt work, withhold final reports, or suspend an analysis for due cause as well as authorize the resumption of work.

### **12.3 EVALUATION OF SIGNIFICANCE AND ACTIONS TAKEN**

For each nonconforming issue reported, an evaluation of its significance and the level of management involvement needed is made. This includes reviewing its impact on the final data, whether or not it is an isolated or systematic issue, and how it relates to any special client requirements.

SOP No. CA-L-S-001 distinguishes between situations when it would be appropriate for the laboratory QA Manager and Laboratory Director (or his/her designee) to make the decision on the need for client notification (written or verbal) and data recall (report revision) and when the decision must be made with the assistance of the ECOs and Corporate Management. Laboratory level decisions are documented and approved using the laboratory's standard nonconformance/corrective action reporting (Section 13) in lieu of the data recall determination form contained in SOP No. CA-L-S-001.

### **12.4 PREVENTION OF NONCONFORMING WORK**

If it is determined that the nonconforming work could recur, further corrective actions must be made following the laboratory's corrective action system (Section 13).

On a monthly basis, the QA Department evaluates non-conformances to determine if any nonconforming work has been repeated multiple times. If so, the laboratory's corrective action process may be followed.

## **12.5 METHOD SUSPENSION/RESTRICTION (STOP WORK PROCEDURES)**

In some cases it may be necessary to suspend/restrict the use of a method or target compound which constitutes significant risk and/or liability to the laboratory. Suspension/restriction procedures can be initiated by any of the persons noted in Section 12.2, Paragraph 5 above.

Prior to suspension/restriction, confidentiality will be respected, and the problem and the required corrective and preventive action will be stated in writing and presented to the Laboratory Director.

The Laboratory Director shall arrange for the appropriate personnel to meet with the QA Manager as needed. This meeting shall be held to confirm that there is a problem, that suspension/restriction of the method is required and will be concluded with a discussion of the steps necessary to bring the method/target or test fully back on line. In some cases that may not be necessary if all appropriate personnel have already agreed there is a problem and there is agreement on the steps needed to bring the method, target or test fully back on line.

The QA Manager will also initiate a corrective action report as described in Section 13 if one has not already been started. A copy of any meeting notes and agreed upon steps should be faxed or e-mailed by the laboratory to the appropriate General Manager and member of Corporate QA. This fax/e-mail acts as notification of the incident.

After suspension/restriction, the lab will hold all reports to clients pending review. No faxing, mailing or distributing through electronic means may occur. The report must not be posted for viewing on the internet. It is the responsibility of the Laboratory Director to hold all reporting and to notify all relevant laboratory personnel regarding the suspension/restriction (i.e., Project Management, Log-in, etc...). Clients will NOT generally be notified at this time. Analysis may proceed in some instances depending on the non-conformance issue.

Within 72 hours, the QA Manager will determine if compliance is now met and reports can be released, OR determine the plan of action to bring work into compliance, and release work. A team, with all principals involved (Laboratory Director, Operations Manager, QA Manager, Department Manager) can devise a start-up plan to cover all steps from client notification through compliance and release of reports. Project Management, the Director of Client Services and Sales and Marketing should be notified if clients must be notified or if the suspension/restriction affects the laboratory's ability to accept work. The QA Manager must approve start-up or elimination of any restrictions after all corrective action is complete. This approval is given by final signature on the completed corrective action report as described in Section 13.

## SECTION 13

### CORRECTIVE ACTION (NELAC 5.4.10)

#### 13.1 OVERVIEW

A major component of TestAmerica's Quality Assurance (QA) Program is the problem investigation and feedback mechanism designed to keep the laboratory staff informed on quality related issues and to provide insight to problem resolution. When nonconforming work or departures from policies and procedures in the quality system or technical operations are identified, the corrective action procedure provides a systematic approach to assess the issues, restore the laboratory's system integrity, and prevent reoccurrence. Corrective actions are documented using Non-Conformance Memos (NCM) (refer to Figure 13-1).

#### 13.2 DEFINITIONS

- **Correction:** Actions necessary to correct or repair analysis specific non-conformances. The acceptance criteria for method specific QC and protocols as well as the associated corrective actions are contained in the method specific SOPs and Appendix 4. The analyst will most frequently be the one to identify the need for this action as a result of calibration checks and QC sample analysis. No significant action is taken to change behavior, process or procedure.
- **Corrective Action:** The action taken is not only a correction made to the immediate event, but a change in process, procedure or behavior that is required to eliminate the causes of an existing nonconformity, defect, or other undesirable situation in order to prevent recurrence.

#### 13.3 GENERAL

Problems within the quality system or within analytical operations may be discovered in a variety of ways, such as QC sample failures, internal or external audits, proficiency testing (PT) performance, client complaints, staff observation, etc.

The purpose of a corrective action system is to:

- Identify non-conformance events and assign responsibility for investigation.
- Resolve non-conformance events and assign responsibility for any required corrective action.
- Identify Systematic Problems before they become serious.
- Identify and track Client complaints and provide resolution (see more on client complaints in Section 11).

**13.3.1 Non-Conformance Memo (NCM)** - is used to document the following types of corrective actions:

- Deviations from an established procedure or SOP
- QC outside of limits (non matrix related)

- Isolated Reporting / Calculation Errors
- Failed or Unacceptable PT results.
- Corrective actions that cross multiple departments in the laboratory.
- Systematic Reporting / Calculation Errors

#### **13.4 CLOSED LOOP CORRECTIVE ACTION PROCESS**

Any employee in the company can initiate a corrective action. There are four main components to a closed-loop corrective action process once an issue has been identified: Cause Analysis, Selection and Implementation of Corrective Actions (both short and long term), Monitoring of the Corrective Actions, and Follow-up.

##### **13.4.1 Cause Analysis**

- Upon discovery of a non-conformance event, the event must be defined and documented. An NCM must be initiated, someone is assigned to investigate the issue and the event is investigated for cause. Laboratory SOP No. WS-QA-0023, Nonconformance and Corrective Action System, provides some general guidelines on determining responsibility for assessment.
- The cause analysis step is the key to the process as a long term corrective action cannot be determined until the cause is determined.
- If the cause is not readily obvious, the Department Manager or QA Manager (or QA designee) is consulted.

##### **13.4.2 Selection and Implementation of Corrective Actions**

- Where corrective action is needed, the laboratory shall identify potential corrective actions. The action(s) most likely to eliminate the problem and prevent recurrence are selected and implemented. Responsibility for implementation is assigned.
- Corrective actions shall be to a degree appropriate to the magnitude of the problem identified through the cause analysis.
- Whatever corrective action is determined to be appropriate, the laboratory shall document and implement the changes. The NCM is used for this documentation.

##### **13.4.3 Monitoring of the Corrective Actions**

- The Department Manager and QA Manager are responsible to ensure that the corrective action taken was effective.
- Ineffective actions will be documented and re-evaluated until acceptable resolution is achieved. Department Managers are accountable to the Laboratory Director to ensure final acceptable resolution is achieved and documented appropriately.
- Each NCM is entered into a database for tracking purposes and reviewed to ensure that the corrective actions have taken effect.
- The QA Manager or designee reviews monthly NCMs for trends. Highlights are included in the QA monthly report (refer to Section 17). If a significant trend develops that adversely affects quality, an audit of the area is performed and corrective action implemented.

- Any out-of-control situations that are not addressed acceptably at the laboratory level may be reported to the Corporate Quality Director by the QA Manager, indicating the nature of the out-of-control situation and problems encountered in solving the situation.

#### **13.4.4 Follow-up Audits**

- Follow-up audits may be initiated by the QA Manager and shall be performed as soon as possible when the identification of a nonconformance casts doubt on the laboratory's compliance with its own policies and procedures, or on its compliance with state or federal requirements. (Section 16 includes additional information regarding internal audit procedures.)
- These audits often follow the implementation of the corrective actions to verify effectiveness. An additional audit would only be necessary when a critical issue or risk to business is discovered.

### **13.5 TECHNICAL CORRECTIVE ACTIONS**

In addition to providing acceptance criteria and specific protocols for technical corrective actions in the method SOPs and Appendix 4, the laboratory has general procedures to be followed to determine when departures from the documented policies and procedures and quality control have occurred (refer to Section 12 for information regarding the control of non-conforming work). The documentation of these procedures is through the use of an NCM.

Appendix 4 includes examples of general technical corrective actions. For specific criteria and corrective actions refer to the analytical methods or specific method SOPs.

Laboratory SOP No. WS-QA-0023, "Nonconformance and Corrective Action System", provides some general guidelines for identifying the individual(s) responsible for assessing each QC type and initiating corrective action. The table also provides general guidance on how a data set should be treated if associated QC measurements are unacceptable. Specific procedures are included in Method SOPs, Appendix 4, QAM Sections 20 and 21, and SOP CA-L-S-001 (Internal Investigation of Potential Data Discrepancies and Determination for Data Recall). All corrective actions are reviewed at a minimum monthly by the QA Manager and highlights are included in the QA monthly report.

To the extent possible, samples shall be reported only if all quality control measures are acceptable. If the deficiency does not impair the usability of the results, data will be reported with an appropriate data qualifier and/or the deficiency will be noted in the case narrative. Where sample results may be impaired, the Project Manager is notified electronically by the NCM program and appropriate corrective action (e.g., reanalysis) is taken and documented.

### **13.6 BASIC CORRECTIONS**

When mistakes occur in records, each mistake shall be crossed-out, and not erased, deleted, made illegible, or otherwise obliterated (e.g. no white-out), and the correct value entered alongside. All such corrections shall be initialed (or signed) and dated by the person making the correction. In the case of records stored electronically, the original "uncorrected" file must be maintained intact and a second "corrected" file is created.


This same process applies to adding additional information to a record. All additions made later than the initial must also be initialed (or signed) and dated.

When corrections are due to reasons other than obvious transcription errors, the reason for the corrections (or additions) shall also be documented.

Figure 13-1.  
Example - Corrective Action Report

CORRECTIVE ACTION REPORT

Example Screens:

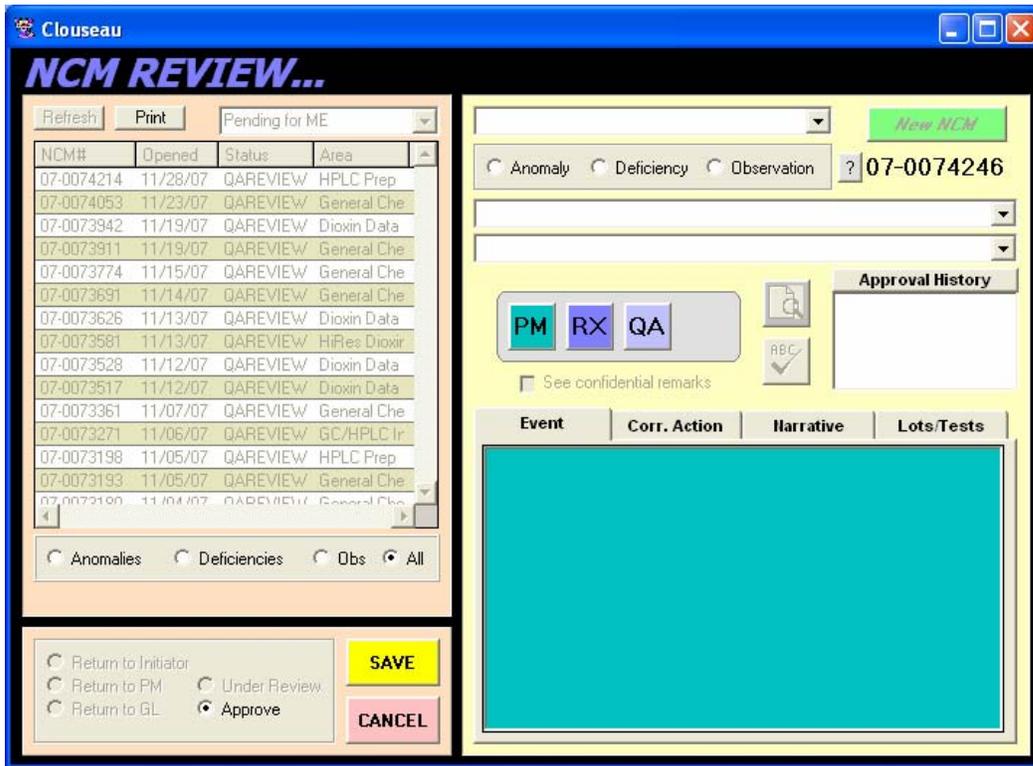

**Clouseau** [Min] [Max] [Close]

## NCM REVIEW...

Refresh
Print
Pending for ME

NCM#	Opened	Status	Area
07-0074214	11/28/07	QAREVIEW	HPLC Prep
07-0074053	11/23/07	QAREVIEW	General Che
07-0073942	11/19/07	QAREVIEW	Dioxin Data
07-0073911	11/19/07	QAREVIEW	General Che
07-0073774	11/15/07	QAREVIEW	General Che
07-0073691	11/14/07	QAREVIEW	General Che
07-0073626	11/13/07	QAREVIEW	Dioxin Data
07-0073581	11/13/07	QAREVIEW	HiRes Dioxir
07-0073528	11/12/07	QAREVIEW	Dioxin Data
07-0073517	11/12/07	QAREVIEW	Dioxin Data
07-0073361	11/07/07	QAREVIEW	General Che
07-0073271	11/06/07	QAREVIEW	GC/HPLC Ir
07-0073198	11/05/07	QAREVIEW	HPLC Prep
07-0073193	11/05/07	QAREVIEW	General Che
07-0073190	11/04/07	QAREVIEW	General Che

Anomalies
 Deficiencies
 Obs
 All

Return to Initiator
 Return to PM
 Return to GL
 Under Review
 Approve
SAVE
CANCEL

?
New NCM

Anomaly
 Deficiency
 Observation
07-0074246

PM
RX
QA

See confidential remarks

Approval History

Event
Corr. Action
Narrative
Lots/Tests

Work Order	Batch	Lot	Smp	Sfx	Mth	ME

Add Associations

**Clouseau** [Min] [Max] [Close]

## NCM REVIEW...

Refresh
Print
Pending for ME

NCM#	Opened	Status	Area
07-0074214	11/28/07	QAREVIEW	HPLC Prep
07-0074053	11/23/07	QAREVIEW	General Che
07-0073942	11/19/07	QAREVIEW	Dioxin Data
07-0073911	11/19/07	QAREVIEW	General Che
07-0073774	11/15/07	QAREVIEW	General Che
07-0073691	11/14/07	QAREVIEW	General Che
07-0073626	11/13/07	QAREVIEW	Dioxin Data
07-0073581	11/13/07	QAREVIEW	HiRes Dioxir
07-0073528	11/12/07	QAREVIEW	Dioxin Data
07-0073517	11/12/07	QAREVIEW	Dioxin Data
07-0073361	11/07/07	QAREVIEW	General Che
07-0073271	11/06/07	QAREVIEW	GC/HPLC Ir
07-0073198	11/05/07	QAREVIEW	HPLC Prep
07-0073193	11/05/07	QAREVIEW	General Che
07-0073190	11/04/07	QAREVIEW	General Chemistry

Anomalies
 Deficiencies
 Obs
 All

Return to Initiator
 Return to PM
 Return to GL
 Under Review
 Approve
SAVE
CANCEL

?
New NCM

Anomaly
 Deficiency
 Observation
?

PM
RX

See confidential remarks

Approval History

Event
Corr. Action
Narrative
Lots/Tests

## SECTION 14.0

### PREVENTIVE ACTION (NELAC 5.4.11)

#### 14.1 OVERVIEW

The laboratory's preventive action programs improve, or eliminate potential causes of nonconforming product and/or nonconformance to the quality system. This preventive action process is a proactive continuous process improvement activity that can be initiated through feedback from clients, employees, business providers, and affiliates. The QA Department has the overall responsibility to ensure that the preventive action process is in place, and that relevant information on actions is submitted for management review.

Dedicating resources to an effective preventive action system emphasizes TestAmerica West Sacramento's commitment to its Quality Assurance (QA) program. It is beneficial to identify and address negative trends before they develop into complaints, problems and corrective actions. Additionally, customer service and satisfaction can be improved through continuous improvements to laboratory systems.

Opportunities for improvement may be discovered during management reviews, the QA Metrics Report, internal or external audits, proficiency testing performance, client complaints, staff observation, etc.

The monthly Quality Assurance Metrics Report shows performance indicators in all areas of the quality system. These areas include revised reports, corrective actions, audit findings, internal auditing and data authenticity audits, client complaints, PT samples, holding time violations, SOPs, ethics training, etc. These metrics are used to help evaluate quality system performance on an ongoing basis and provide a tool for identifying areas for improvement.

The laboratory's Corrective Action process (Section 13) is integral to implementation of preventive actions. A critical piece of the corrective action process is the implementation of actions to prevent further occurrence of a non-compliance event. Historical review of corrective action provides a valuable mechanism for identifying preventive action opportunities.

**14.1.1** The following elements are part of a preventive action system:

- Identification of an opportunity for preventive action.
- Process for the preventive action.
- Define the measurements of the effectiveness of the process once undertaken.
- Execution of the preventive action.
- Evaluation of the plan using the defined measurements.
- Verification of the effectiveness of the preventive action.
- Close-Out by documenting any permanent changes to the Quality System as a result of the Preventive Action. Documentation of Preventive Action is incorporated into the monthly QA reports, corrective action process, and management review.

**Note:** There may be varying levels of formality and documentation during the preventive action process due to the simplicity/complexity of the action taken.

**14.1.2** Any Preventive Actions undertaken or attempted shall be taken into account during the Annual Management Review (Section 17). A highly detailed recap is not required; a simple recount of success and failure within the preventive action program will provide management a measure for evaluation.

**SECTION 15.0**

**CONTROL OF RECORDS  
(NELAC 5.4.12)**

TestAmerica West Sacramento maintains a record system appropriate to its needs and that complies with applicable standards or regulations as required. The system produces unequivocal, accurate records that document all laboratory activities. The laboratory retains all original observations, calculations and derived data, calibration records and a copy of the analytical report for a minimum of five years after it has been issued. Refer to SOP No. WS-QA-0009, "Document Archiving", for specific details.

**15.1 OVERVIEW**

The laboratory has established procedures for identification, collection, indexing, access, filing, storage, maintenance and disposal of quality and technical records. A record index is listed in Table 15-1. Quality records are maintained by the Quality Assurance (QA) Manager in a database, which is backed up as part of the regular network backup. Records are of two types; either electronic or hard copy paper formats depending on whether the record is computer or hand generated (some records may be in both formats). Technical records are maintained by Department Managers.

**Table 15-1. Record Index<sup>1</sup>**

Technical Records	Official Documents	QA Records	Project Records	Administrative Records
<b>Retention:</b> 5 Years from analytical report issue*	5 Years from document retirement date*	5 Years from archival* <b>Data Investigation:</b> 5years or the life of the affected raw data storage whichever is greater (beyond 5 years if ongoing project or pending investigation)	5 Years from analytical report issue*	<b>Personnel:</b> 7 Years (HR Records must be maintained as per Policy CW-L-P-001) <b>Finance:</b> See Accounting and Control Procedures Manual
Raw Data	Quality Assurance Manual (QAM)	Internal and External Audits/ Responses	Sample receipt and COC Documentation	Finance and Accounting
Logbooks <sup>2</sup>	Work Instructions	Certifications	Contracts and Amendments	EH&S Manual, Permits, Disposal Records <sup>3</sup>
Standards	SOPs	Corrective/Preventive Action	Correspondence	Employee Handbook
Certificates	Manuals	Management Reviews	QAPP	Personnel files, Employee Signature & Initials, Administrative Training Records (e.g., Ethics)
Analytical Records		Method & Software Validation, Verification data	SAP	
Lab Reports		Data Investigation	Telephone Logbooks	Administrative Policies

Technical Records	Official Documents	QA Records	Project Records	Administrative Records
<b>Retention:</b> 5 Years from analytical report issue*	5 Years from document retirement date*	5 Years from archival* <b>Data Investigation:</b> 5years or the life of the affected raw data storage whichever is greater (beyond 5 years if ongoing project or pending investigation)	5 Years from analytical report issue*	<b>Personnel:</b> 7 Years (HR Records must be maintained as per Policy CW-L-P-001) <b>Finance:</b> See Accounting and Control Procedures Manual
	Policies		Lab Reports	Technical Training Records

<sup>1</sup> Record Types encompass hardcopy and electronic records.

<sup>2</sup> Examples of Logbook types: Maintenance, Instrument Run, Preparation (standard and samples), Standard and Reagent Receipt, Archiving, Balance Calibration, Temperature (hardcopy or electronic records).

<sup>3</sup> Maintained indefinitely.

\* Exceptions listed in Table 15-2.

All records are legible and stored and retained in such a way that they are secure and readily retrievable at the laboratory facility or the Iron Mountain data storage facility that provides a suitable environment to prevent damage or deterioration and to prevent loss. Retention of records are maintained on-site at the laboratory for at least 1 month after their generation and moved offsite for the remainder of the required storage time. Records are maintained for a minimum of five years unless other wise specified by a client or regulatory requirement.

For raw data and project records, record retention shall be calculated from the date the project report is issued. For other records, such as Controlled Documents, QA, or Administrative Records, the retention time is calculated from the date the record is formally retired. Records related to the programs listed in Table 15-2 have lengthier retention requirements and are subject to the requirements in Section 15.1.3. Policy CW-L-P-001 (Record Retention) provides additional information on record retention requirements.

### 15.1.1 Programs with Longer Retention Requirements

Some regulatory programs have longer record retention requirements than the standard record retention time. These are detailed in Table 15-3 with their retention requirements. In these cases, the longer retention requirement is enacted. If special instructions exist such that client data cannot be destroyed prior to notification of the client, the container or box containing that data is marked as to who to contact for authorization prior to destroying the data.

**Table 15-2. Special Record Retention Requirements**

<b>Program</b>	<b><sup>1</sup>Retention Requirement</b>
Drinking Water – All States	10 years (project records)
Drinking Water Lead and Copper Rule	12 years (project records)
Commonwealth of MA – All environmental data 310 CMR 42.14	10 years
FIFRA – 40 CFR Part 160	Retain for life of research or marketing permit for pesticides regulated by EPA
Housing and Urban Development (HUD) Environmental Lead Testing	10 years
Alaska	10 years
Louisiana – All	10 years
Michigan Department of Environmental Quality – all environmental data	10 years
NY Potable Water NYCRR Part 55-2	10 years
TSCA - 40 CFR Part 792	10 years after publication of final test rule or negotiated test agreement

<sup>1</sup>Note: Extended retention requirements must be noted with the archive documents or addressed in facility-specific records retention procedures.

**15.1.2** All records are held secure and in confidence. Records maintained at the laboratory are located in the data archive room. Records archived off-site are stored in a secure location where a record is maintained of any entry into the storage facility. Logs are maintained in a logbook to note removal and return of records.

**15.1.3** The laboratory has procedures to protect and back-up records stored electronically and to prevent unauthorized access to or amendment of these records. All analytical data is maintained as hard copy or in a secure readable electronic format. For analytical reports that are maintained as copies in PDF format, see section 20.12.1 ‘Computer and Electronic Data Related Requirements’ for more information.

**15.1.4** The record keeping system allows for historical reconstruction of all laboratory activities that produced the analytical data, as well as rapid recovery of historical data (Records stored off site should be accessible within 2 days of a request for such records). The history of the sample from when the laboratory took possession of the samples must be readily understood through the documentation. This shall include inter-laboratory transfers of samples and/or extracts.

- The records include the identity of personnel involved in sampling, sample receipt, preparation, or testing. All analytical work contains the initials (at least) of the personnel involved. The laboratory’s copy of the chain of custody is stored with the invoice and the work order sheet generated by the LIMS. The chain of custody would indicate the name of the sampler. If any sampling notes are provided with a work order, they are kept with this package.

- All information relating to the laboratory facilities equipment, analytical test methods, and related laboratory activities, such as sample receipt, sample preparation, or data verification are documented.
- The record keeping system facilitates the retrieval of all working files and archived records for inspection and verification purposes (e.g., set format for naming electronic files, set format for what is included with a given analytical data set. Refer to SOP WS-QA-0009, "Document Archiving". Instrument data is stored by project, except for inorganics, and calibration data. Inorganics and calibration data is stored sequentially by instrument as appropriate.
- Changes to hardcopy records shall follow the procedures outlined in Section 13 and 20. Changes to electronic records in LIMS or instrument data are recorded in audit trails.
- The reason for a signature or initials on a document is clearly indicated in the records such as "sampled by," "prepared by," "reviewed by", or "Analyzed by".
- All generated data except those that are generated by automated data collection systems, are recorded directly, promptly and legibly in permanent dark ink.
- Hard copy data may be scanned into PDF format for record storage as long as the scanning process can be verified in order to ensure that no data is lost and the data files and storage media must be tested to verify the laboratory's ability to retrieve the information prior to the destruction of the hard copy that was scanned.
- Also refer to Section 20.13.1 'Computer and Electronic Data Related Requirements'.

## **15.2 TECHNICAL AND ANALYTICAL RECORDS**

**15.2.1** The laboratory retains records of original observations, derived data and sufficient information to establish an audit trail, calibration records, staff records and a copy of each analytical report issued, for a minimum of five years unless otherwise specified by a client or regulatory requirement (refer to Section 15.1). The records for each analysis shall contain sufficient information to enable the analysis to be repeated under conditions as close as possible to the original. The records shall include the identity of laboratory personnel responsible for the sampling, performance of each analysis and checking of results.

**15.2.2** Observations, data and calculations are recorded at the time they are made and are identifiable to the specific task.

**15.2.3** Changes to hardcopy records shall follow the procedures outlined in Section 13 and 20. Changes to electronic records in LIMS or instrument data are recorded in audit trails. The essential information to be associated with analysis, such as strip charts, tabular printouts, computer data files, analytical notebooks, and run logs, include (previous discussions relate where most of this information is maintained – specifics may be added below):

- laboratory sample ID code;
- Date of analysis and time of analysis is required if the holding time is seventy-two (72) hours or less, or when time critical steps are included in the analysis (e.g., drying times,

incubations, etc.); instrumental analyses have the date and time of analysis recorded as part of their general operations. Where a time critical step exists in an analysis, location for such a time is included as part of the documentation on a benchsheet or in the LIMS.

- Instrumentation identification and instrument operating conditions/parameters. Operating conditions/parameters are typically recorded in instrument maintenance logs where available.
- analysis type;
- all manual calculations and manual integrations;
- analyst's or operator's initials/signature;
- sample preparation including cleanup, separation protocols, incubation periods or subculture, ID codes, volumes, weights, instrument printouts, meter readings, calculations, reagents;
- test results;
- standard and reagent origin, receipt, preparation, and use;
- calibration criteria, frequency and acceptance criteria;
- data and statistical calculations, review, confirmation, interpretation, assessment and reporting conventions;
- quality control protocols and assessment;
- electronic data security, software documentation and verification, software and hardware audits, backups, and records of any changes to automated data entries; and
- Method performance criteria including expected quality control requirements. These are indicated both in the LIMS and on specific analytical report formats.

### **15.3 LABORATORY SUPPORT ACTIVITIES**

In addition to documenting all the above-mentioned activities, the following are retained QA records and project records (previous discussions in this section relate where and how these data are stored):

- all original raw data, whether hard copy or electronic, for calibrations, samples and quality control measures, including analysts' work sheets and data output records (chromatograms, strip charts, and other instrument response readout records);
- a written description or reference to the specific test method used which includes a description of the specific computational steps used to translate parametric observations into a reportable analytical value;
- copies of final reports;
- archived SOPs;
- correspondence relating to laboratory activities for a specific project;
- all corrective action reports, audits and audit responses;
- proficiency test results and raw data; and
- results of data review, verification, and crosschecking procedures

### **15.3.1 Sample Handling Records**

Sample handling and tracking is discussed in Section 24. Records of all procedures to which a sample is subjected while in the possession of the laboratory are maintained. These include but are not limited to records pertaining to:

- sample preservation including appropriateness of sample container and compliance with holding time requirement;
- sample identification, receipt, acceptance or rejection and login;
- sample storage and tracking including shipping receipts, sample transmittal / COC forms; and
- procedures for the receipt and retention of samples, including all provisions necessary to protect the integrity of samples.

### **15.4 ADMINISTRATIVE RECORDS**

The laboratory also maintains the administrative records in either electronic or hard copy form. See Table 15-1.

### **15.5 RECORDS MANAGEMENT, STORAGE AND DISPOSAL**

**15.5.1** All records (including those pertaining to test equipment), certificates and reports are safely stored, held secure and in confidence to the client. Certification related records are available to the accrediting body upon request.

**15.5.2** All information necessary for the historical reconstruction of data is maintained by the laboratory. Records that are stored only on electronic media must be supported by the hardware and software necessary for their retrieval.

**15.5.3** Records that are stored or generated by computers or personal computers have hard copy, write-protected backup copies, or an electronic audit trail controlling access.

**15.5.4** TestAmerica West Sacramento has a record management system for control of laboratory notebooks, instrument logbooks, standards logbooks, and records for data reduction, validation, storage and reporting. Laboratory notebooks are issued by the QA Department and are numbered sequentially. No analysis has more than one active notebook at a time, so all data are recorded sequentially within a series of sequential notebooks. Bench sheets are filed with the data. Standards are maintained in a logbook or using the Veritas Electronic Standards Logbook.

**15.5.5** Records are considered archived when moved to the data archive room. Access to archived hard-copy information is documented with an access log and in/out records is used in archived boxes to note data that is removed and returned. All records shall be protected against fire, theft, loss, environmental deterioration, and vermin. In the case of electronic records, electronic or magnetic sources, storage media are protected from deterioration caused by magnetic fields and/or electronic deterioration. Access to the data is limited to laboratory and

company employees.

**15.5.6** In the event that the laboratory transfers ownership or goes out of business, TestAmerica West Sacramento shall ensure that the records are maintained or transferred according to client's instructions. Upon ownership transfer, record retention requirements shall be addressed in the ownership transfer agreement and the responsibility for maintaining archives is clearly established. In addition, in cases of bankruptcy, appropriate regulatory and state legal requirements concerning laboratory records must be followed. In the event of the closure of the laboratory, all records will revert to the control of the corporate headquarters. Should the entire company cease to exist, as much notice as possible will be given to clients and the accrediting bodies who have worked with the laboratory during the previous 5 years of such action.

**15.5.7 Records Disposal**

**15.5.7.1** Records are removed from the archive and disposed after 5 years unless otherwise specified by a client or regulatory requirement. On a project specific or program basis, clients may need to be notified prior to record destruction. Records are destroyed in a manner that ensures their confidentiality such as shredding, mutilation or incineration.

**15.5.7.2** Electronic copies of records must be destroyed by erasure or physically damaging off-line storage media so no records can be read.

**15.5.7.3** If a third party records management company is hired to dispose of records, a "Certificate of Destruction" is required. [Refer to Policy No. CW-L-P-001 (Records Retention).]

## SECTION 16

### AUDITS (NELAC 5.4.13)

#### 16.1 OVERVIEW

Audits measure laboratory performance and insure compliance with accreditation/certification and project requirements. Audits specifically provide management with an on-going assessment of the quality of results produced by the laboratory, including how well the policies and procedures of the QA system and the Ethics and Data Integrity Program are being executed. They are also instrumental in identifying areas where improvement in the QA system will increase the reliability of data. There are two principle types of audits: Internal and External. Internal audits are performed by laboratory or corporate personnel. External audits are conducted by regulators, clients or third-party auditing firms. In either case, the assessment to program requirements is the focus.

**Table 16-1. Audit Types and Frequency**

Internal Audits	Description	Performed by	Frequency
	Analyst & Method Compliance	QA Department or Designee	- 100% of all methods over a two year period. - 100% of all analysts annually.
	Instrument	QA Department or Designee	100% of all organic instruments and any inorganic chromatography instruments. Over a two year period.
	Work Order/ Final Report	QA Department or Designee	- 1 complete report each month.
	Support Systems	QA Department or Designee	- Annual for entire labs support departments & equipment (e.g., thermometers, balances), can be divided into sub-sections over the course of the year.
	Performance Audits (Double-Blind PTs)	Corporate QA, Laboratory QA Department or Designee	- As needed.
	Special	QA Department or Designee	- As Needed
External Audits	Description	Performed by	Frequency
	Program / Method Compliance	Regulatory Agencies, Clients, accreditation organizations	- As required by program and/or clients needs
	Performance Audits	Provided by a third party.	- As required by a client or regulatory agency. Generally provided semi-annually through the analysis of PT samples.

#### 16.2 INTERNAL AUDITS

Annually, the laboratory prepares a schedule of internal audits to be performed throughout the year. As previously stated, these audits verify and monitor that operations continue to comply with the requirements of the laboratory's QA Manual, the Corporate Ethics Program, DoD QSM

and NELAC. A schedule of the internal audits is maintained by the QA Manager in the *Internal Audit Workbook*. An example can be found in Attachment 1.

It is the responsibility of the QA Manager to plan and organize audits in consideration of the laboratory work load and the department personnel schedules so that all pertinent personnel and operations are thoroughly reviewed. When designees (other than QA department personnel & approved by the QA Manager), perform audits, the QA Manager shall insure that these persons do not audit their own activities except when it can be demonstrated that an effective audit will be carried out. In general, the auditor:

- Is neither the person responsible for the process being audited nor the immediate supervisor of the person responsible for the project/process.
- Is free of any conflicts of interest.
- Is free from bias and influences that could affect objectivity.

Laboratory personnel (e.g., supervisors and analysts) may assist with both method and support system audits as long as the items listed in the above paragraph are observed. These audits are conducted according to defined criteria listed in the checklists of the *Internal Audit Workbook*. These personnel must be approved by the QA Manager; and must complete the audit checklists in their entirety. This process introduces analyst experience and insight into the laboratory's auditing program.

The auditor must review the previous audit report and identify all items for verification of corrective actions. A primary focus will be dedicated to the ability of the laboratory to correct root-cause deficiencies and that the corrective action has been implemented and sustained as documented.

### **16.2.1 Systems**

An annual systems audit is required to ensure compliance to analytical methods and SOPs, the laboratory's Data Integrity and Ethics Policies, NELAC quality systems, client and State requirements. This audit is performed in portions throughout the year through method, analyst, instrument, work order/final report and support system audits. Audits are documented and reported to management within 1 week of their performance. Systems audits cover all departments of the facility, both operational and support. The multiple audits are compiled into one systems audit package at the end of the year (*Internal Audit Workbook*).

#### **16.2.1.1 Method, Analyst, Instrument and Work Order/Final Report Audits**

Procedures for the method compliance, analyst, instrument and work order/final report audits are incorporated by reference to SOP No. CA-Q-S-004, Method Compliance and Data Authenticity Audits. These audits are not mutually exclusive. For example, the performance of a method audit will also cover multiple analysts and instruments. The laboratory's goal is to review all analysts and instruments as described in SOP No. CA-Q-S-004. The laboratory will also audit all methods within a two year time period and audit a minimum of one Work Order/Final Report from receiving through reporting on a monthly basis.

#### **16.2.1.2 Support Systems**

Support system audits are performed to ensure that all departments & ancillary equipment are operating according to prescribed criteria. Support system audits include the review of both non-analytical and operational departments. Support equipment audits (e.g., metrology items) include the review of balance calibrations, weight calibrations; water quality testing, etc. Non-analytical may include sample receiving and bottle preparation. These types of support audits ensure that the operations are being performed to support ethical data as well as ensuring the accuracy & precision of the utilized equipment.

These audits can be performed in portions throughout the year or in one scheduled session. However, the audit schedule must document that these aspects are reviewed annually. Many of the metrology systems are considered to be surveillance activities that can be monitored by QA personnel or delegated to specified department personnel. These surveillance activities are performed on a semi-annual basis unless issues warrant a greater frequency or previous audits continually showing no deficiencies allow the frequency to be reduced to once a year.

An example audit checklist can be found in Attachment 2. Instructions for reporting findings are included in the *Internal Audit Workbook*. In general, findings are reported to management within 1 week of the audit and a response is due from management within 30 days.

#### **16.2.2 Performance Audits**

Corporate QA may arrange for double blind PT studies to be performed in the laboratories. Results are given to Management and Corrective actions of any findings are coordinated at each facility by the QA Managers and Laboratory Directors/Managers. These studies are performed on an as needed basis. They may be performed when concerns are raised regarding the performance of a particular method in specific laboratories, periodically to evaluate methods that may not normally be covered in the external PT program or may be used in the process of developing best practices. The local QA Manager may also arrange for PT studies on an as needed basis. (Refer to Section 16.3.2 for additional information on Performance Audits.)

#### **16.2.3 Special Audits**

Special audits are conducted on an as needed basis, generally as a follow up to specific issues such as client complaints, corrective actions, PT results, data audits, system audits, validation comments, regulatory audits or suspected ethical improprieties. Special audits are focused on a specific issue, and report format, distribution, and timeframes are designed to address the nature of the issue.

### **16.3 EXTERNAL AUDITS**

TestAmerica facilities are routinely audited by clients and external regulatory authorities. External audits are performed when certifying agencies or clients conduct on-site inspections or submit performance testing samples for analysis. It is TestAmerica's policy to cooperate fully with regulatory authorities and clients. The laboratory makes every effort to provide the auditors with access to personnel, documentation, and assistance. The department managers are responsible for providing corrective actions to the QA Manager who coordinates the response

for any deficiencies discovered during an external audit. Audit responses are due in the time allotted by the client or agency performing the audit. This time frame is generally 30 days.

TestAmerica West Sacramento cooperates with clients and their representatives to monitor the laboratory's performance in relation to work performed for the client. The client may only view data and systems related directly to the client's work. All efforts are made to keep other client information confidential.

### **16.3.1 Confidential Business Information (CBI) Considerations**

During on-site audits, on-site auditors may come into possession of information claimed as business confidential. A business confidentiality claim is defined as "a claim or allegation that business information is entitled to confidential treatment for reasons of business confidentiality or a request for a determination that such information is entitled to such treatment." When information is claimed as business confidential, the laboratory must place on (or attach to) the information at the time it is submitted to the auditor, a cover sheet, stamped or typed legend or other suitable form of notice, employing language such as "trade secret", "proprietary" or "company confidential". Confidential portions of documents otherwise non-confidential must be clearly identified. CBI may be purged of references to client identity by the responsible laboratory official at the time of removal from the laboratory. However, sample identifiers may not be obscured from the information. Additional information regarding CBI can be found within the 2003 NELAC standards.

### **16.3.2 Performance Audits**

The laboratory is involved in performance audits conducted semi-annually through the analysis of PT samples provided by a third party. The laboratory generally participates in the following types of PT studies: Soil, Water Supply, Water Pollution, Air, and round-robin studies for sediments and biological materials.

- It is TestAmerica's policy that PT samples be treated as typical samples in the production process. Further, where PT samples present special or unique problems in the regular production process they may need to be treated differently, as would any special or unique request submitted by any client. The QA Manager must be consulted and in agreement with any decisions made to treat a PT sample differently due to some special circumstance.
- PTs generally do not have holding times associated with them. In the absence of any holding time requirement, it is recommended that the holding time begin when the PT sample is prepared according to the manufacturers instructions. Holding times should apply to full volume PT samples only if the provider gives a meaningful "sampling date". If this is not provided, it is recommended that the date/time of opening of the full volume sample be considered the beginning of holding time.
- Login will obtain the COC information from the documentation provided with the PTs with review by QA or other designated staff.
- Vials will be prepared as required in the instruction set provided with the samples. After preparation to full volume the sample may be spiked, digested, concentrated, etc., as would be done for any normal sample requiring similar analysis.

- PT samples will not undergo multiple preps, multiple runs, multiple methods (unless being used to evaluate multiple methods), multiple dilutions, UNLESS this is what would be done to a normal client sample (e.g. if a client requests, as PT clients do, that we split VOA coeluters, then dual analysis IS normal practice).
- The type, composition, concentration and frequency of quality control samples analyzed with the PT samples shall be the same as with routine environmental samples.
- Instructions may be included in the laboratory's SOPs for how low level samples are analyzed, including concentration of the sample or adjustment of the normality of titrant. When a PT sample falls below the range of the routine analytical method, the low-level procedure may be used.
- No special reviews shall be performed by operations and QA, UNLESS this is what would be done to a normal client sample. To the degree that special report forms or login procedures are required by the PT supplier, it is reasonable that the laboratory WOULD apply special review procedures, as would be done for any client requesting unusual reporting or login processes.
- Written responses to unacceptable PT results are required. In some cases it may be necessary for blind QC samples to be submitted to the laboratory to show a return to control.

#### **16.4      AUDIT FINDINGS**

Internal or External Audit findings should be documented using the corrective action process and database (refer to Section 13). The laboratory is expected to prepare a response to audit findings within 30 days of receipt of an audit report unless the report specifies a different time frame. The response may include action plans that could not be completed within the 30 day timeframe. In these instances, a completion date must be set and agreed to by operations management and the QA Manager.

Responsibility for developing and implementing corrective actions to findings is the responsibility of the Department Manager where the finding originated. Findings that are not corrected by specified due dates are reported monthly to management in the QA monthly report.

If any audit finding casts doubt on the effectiveness of the operations or on the correctness or validity of the laboratory's test results, the laboratory shall take timely corrective action, and shall notify clients in writing if the investigations show that the laboratory results have been affected. Once corrective action is implemented, a follow-up audit is scheduled to ensure that the problem has been corrected.

The procedures must be in accordance to SOP No. CA-L-S-001, Internal Investigations of Data Discrepancies and Determination of Data Recall.

Clients must be notified promptly in writing, of any event such as the identification of defective measuring or test equipment that casts doubt on the validity of results given in any test report or amendment to a test report. The investigation must begin within 24-hours of discovery of the

problem and all efforts are made to notify the client within two weeks after the completion of the investigation.

Figure 16-1.

Example - Internal Audit Workbook

**TestAmerica**  
 THE LEADER IN ENVIRONMENTAL TESTING

TestAmerica <Name>  
 Last Updated: 9/10/2007

Workbook Instruction No. CA-Q-WI-011

**Internal Audit Workbook  
 Summary Page**

Note: Click on the (Summary Page) to located on each audit sheet to return to this page.  
 \* The lab may choose to audit these areas with each method/analyst/instrument audit. The auditor must document on the checklist that this item is audited as part of the <defined> audit.

Area Audited	Audit Type	Audit Cycle	Scheduled	Date Audited	Date Closed	Comments
1 Balances	System	6 mo				
2 Temperature Logs/Thermometers	System	6 mo				
3 Sample Storage and Disposal	System	1yr				
4 Maintenance Logs	System	6 mo				
5 Volatile Storage Blanks	System	6 mo				
6 Lab Water Quality Testing	System	6 mo				
7 Sample Log In	System	1yr				
8 Shipping Procedures	System	1yr				
9 Computer Operations (LIMS)	System	1yr				Pending Corp. IT Policies
10 SOP & Document Distribution System	System	1yr				
11 Archiving Electronic & Paper Records	System	1yr				Pending Corp. IT Policies
12 Statistical Process Control	System	1yr				
13 Data Review System	System	1yr				
14 Final Report Generation	System	1yr				
15 Standards/Reagents	System	6 mo				
16 Manual Integration	System	1yr				
17 Corrective Action System	System	1yr				
18 Training Records	System	6 mo				
19 MDLs	System	1yr				
20 SOPs - Prep/Review/Update Process	System	1yr				
21 Purchasing/Procurement	System	1yr				
22 Eppendorf/Diluter/Dispenser Calibration Check	System	6 mo				
23 Subcontract Lab Approval	System	1yr				
24 Customer Complaint System	System	1yr				
25 Methods	Method	2 yr				

Figure 16-2.

Example – Internal Audit System Checklist: Corrective Actions



(Summary Page)

TestAmerica <Location>

INTERNAL AUDIT - Corrective Actions

[ Printed Name(s) or Date(s) ]

Area Audited: \_\_\_\_\_  
 Auditor: \_\_\_\_\_  
 Date: \_\_\_\_\_  
 Persons Contacted During Audit: \_\_\_\_\_  
 Date Reported to Department Manager: \_\_\_\_\_  
 Reported To: \_\_\_\_\_  
 Date Reported to Lab Director/Manager: \_\_\_\_\_  
 Reported To: \_\_\_\_\_  
 Date Response Due: \_\_\_\_\_  
 Response Received and Accepted by QA Manager: \_\_\_\_\_  
 Associated Corrective Action Report Number(s): \_\_\_\_\_  
 Scheduled Follow-up: \_\_\_\_\_

Item	Requirement	Ref.	Y	N	NA	Evidence/Comments	Follow Up	
1	Does the laboratory have a corrective action program in place?	5.4.10.1						
2	Does the laboratory have a current corrective action SOP or is this information in the QA Manual?	5.4.10.1						
3	Do all laboratory personnel have documented training and access to initiate corrective actions?	5.4.10.1						
4	Are causes clearly identified by department, staff name, scope of issue (how many reports affected)?	5.4.10.6						
5	Is a root cause for the issue identified?	5.4.10.2						
6	Is a corrective action (plan) clearly described?							
7	Was the corrective action fully implemented?							
8	Is documentation (if applicable) completed as specified by the corrective action (training, revised SOP, etc)							
9	Has a follow-up assessment been conducted to verify the corrective action was successful?							
10	Are corrective actions reviewed on a regular basis by management?	5.4.10.6a 5						
11	Is there a defined distribution flow for corrective action notification, review, closure, and follow-up?	5.4.10.6a						
12	Are non-conformances reviewed on a regular basis and used, if necessary, to initiate root cause corrective actions?							
13	Does the lab have a documented procedure for QC corrective action (i.e., documented within each method / parameter SOP or in the QA Manual)?	4.10.1						
14	<b>Verify Corrective Actions from previous systems audits. List Items:</b>							
15								
16								
17								

Auditor Signature: \_\_\_\_\_

Primary Reference(s): Corporate SOP CA-Q-S-002, Acceptable Manual Integration Practices  
 NELAC Standard, June 2003  
 DoD Quality Systems Manual, Version 3, January 2006  
 EPA Manual for the Certification of Laboratories Analyzing Drinking Water

## SECTION 17

### MANAGEMENT REVIEWS (NELAC 5.4.14)

#### 17.1 QUALITY ASSURANCE REPORT

A comprehensive QA Report shall be prepared each month by the laboratory's QA Department and forwarded to the Laboratory Director for review and comments. The final report shall be submitted to the laboratory senior staff as well as the appropriate Quality Director and General Manager. All aspects of the QA system are reviewed to evaluate the suitability of policies and procedures. At a minimum, the report content will contain the items listed below. During the course of the year, the Laboratory Director, General Manager or Corporate QA may request that additional information be added to the report.

The TestAmerica QA Report template is comprised of a discussion of three key QA issues facing the laboratory and ten specific sections (Figure 17-1):

- **Metrics:** Describe actions or improvement activities underway to address any outlying quality metrics that have been reported in the monthly Quality System Metrics Table.
- **SOPs:** Report SOPs that have been finalized and report status of any outstanding SOP reviews.
- **Corrective Actions:** Describe highlights and the most frequent cause for report revisions and corrective/preventive action measures underway. Include a discussion of any recalls handled at the lab level as per Section 6.2.2 in the Investigation/Recall SOP (SOP: CA-L-S-001). Include a section for client feedback and complaints. Include both positive and negative feedback. Describe the most serious client complaints and resolutions in progress.
- **MDLs and Control Limits:** Report which MDLs/ MDL verifications are due. Report the same for Control Limits.
- **Audits:** Report Internal and External Audits that were conducted. Include all relevant information such as which methods, by whom, corrective actions needed by when and discuss unresolved audit findings.
- **Performance Testing (PT) Samples:** Report the PT tests that are currently being tested with their due dates, report recent PT results by study, acceptable, total reported and the month and year.
- **Certifications:** Report on any certification programs being worked on by due date, packages completed. Describe any issues, lapses, or potential revocations.
- **Regulatory Updates:** Include information on new state or federal regulations that may impact the laboratory. Report new methods that require new instrumentation, deletion of methods, changes in sampling requirements and frequencies etc...
- **Miscellaneous:** Include any issues that may impact quality within the laboratory.
- **Next Month:** Report on plans for the upcoming month.
- **Lab Director Comments Section:** This section gives the Laboratory Director the opportunity to comment on issues discussed in the report and to document plans to resolve

these issues. Unresolved issues that reappear in subsequent monthly reports must be commented on by the Laboratory Director.

- **Quality System Metrics Table:** The report also includes statistical results that are used to assess the effectiveness of the quality system. Effective quality systems are the responsibility of the entire laboratory staff. Each laboratory provides their results in a template provided by Corporate QA (Figure 17-2).

On a monthly basis, Corporate QA compiles information from all the monthly laboratory reports. The VP-QA/EHS prepares a report that includes a compilation of all metrics and notable information and concerns regarding the QA programs within the laboratories. The report also includes a listing of new regulations that may potentially impact the laboratories. This report is presented to the Analytical Division Senior Management Team and General Managers.

## **17.2 ANNUAL MANAGEMENT REVIEW**

The senior lab management team (Laboratory Director, Technical Directors, QA Manager, Operations Manager, Manager of Project Management, and Manager of Customer Services) conducts an annual review of its quality systems and LIMS to ensure its continuing suitability and effectiveness in meeting client and regulatory requirements and to introduce any necessary changes or improvements. Corporate Operations and Corporate QA personnel may be included in this meeting at the discretion of the Laboratory Director. The LIMS review consists of examining any audits, complaints or concerns that have been raised through the year that are related to the LIMS. The laboratory will summarize any critical findings that can not be solved by the lab and report them to Corporate IT.

This review uses information generated during the preceding year to assess the “big picture” by ensuring that routine quality actions taken and reviewed on a monthly basis are not components of larger systematic concerns. The monthly review (refer to Section 17.1) should keep the quality systems current and effective, therefore, the annual review is a formal senior management process to review specific existing documentation. Significant issues from the following documentation are compiled or summarized by the QA Manager prior to the review meeting:

- Matters arising from the previous annual review.
- Prior Monthly QA Reports issues.
- Laboratory QA Metrics.
- Review of report reissue requests.
- Review of client feedback and complaints.
- Issues arising from any prior management or staff meetings.
- Minutes from prior Senior Management team meetings. Issues that may be raised from these meetings include:
  - Adequacy of staff, equipment and facility resources.
  - Adequacy of policies and procedures.
  - Future plans for resources and testing capability and capacity.

- The annual internal double blind PT program sample performance (if performed),
- Compliance to the Ethics Policy and Data Integrity Plan. Including any evidence/incidents of inappropriate actions or vulnerabilities related to data Integrity.

The annual review includes the previous 12 months. Based on the annual review, a report is generated by the QA Manager and management. The report is distributed to the appropriate General Manager and the Quality Director. The report includes, but is not limited to:

- The date of the review and the names and titles of participants.
- A reference to the existing data quality related documents and topics that were reviewed.
- Quality system or operational changes or improvements that will be made as a result of the review [e.g., an implementation schedule including assigned responsibilities for the changes (Action Table)].

The QA Manual is also reviewed at this time and revised to reflect any significant changes made to the quality systems.

### **17.3 POTENTIAL INTEGRITY RELATED MANAGERIAL REVIEWS**

Potential integrity issues (data or business related) must be handled and reviewed in a confidential manner until such time as a follow-up evaluation, full investigation, or other appropriate actions have been completed and issues clarified. The Corporate Data Investigation/ Recall SOP shall be followed (SOP No. CA-L-S-001). All investigations that result in finding of inappropriate activity are documented and include any disciplinary actions involved, corrective actions taken, and all appropriate notifications of clients.

The Chairman/CEO, President/CEO, COOs and Quality Directors receive a monthly report from the VP of Quality and EHS summarizing any current data integrity or data recall investigations as described in SOP No. CA-L-S-001. The General Manager's are also made aware of progress on these issues for their specific labs.

**Figure 17-1.**

**Example - QA Monthly Report to Management**

LABORATORY: x  
PERIOD COVERED: Month/Year  
PREPARED BY: x      DATE: Month Day, Year  
DISTRIBUTED TO: xx (Include LD, GM, QA Director, etc...)

THREE KEY ISSUES FOR MONTH:

*Include a discussion of three key issues that were focused in on this month.*

1. x
  2. x
  3. x
- 

**1. METRICS**

*Describe actions or improvement activities underway to address any outlying quality metrics.*

**2. SOPs**

See Tab for SOP specifics.

The following SOPs were finalized (or reviewed for accuracy): (See Tab)

The following SOPs are due to QA: xx

In QA to complete: xx

**3. CORRECTIVE ACTION**

Highlights: xx

Revised Reports:

*Describe the most frequent cause for report revisions and corrective/preventive action measures underway.*

Data Investigations/Recalls (Corporate Data Investigation/Recall SOP):

*Include a discussion of any recalls handled at the lab level as Corp SOP.*

Client Feedback and Complaints:

*Include both positive and negative feedback.*

Describe the most serious client complaints) and resolutions in progress.

**4. MDLs AND CONTROL LIMITS**

MDLs Due:

Control Limits Due:

**5. AUDITS**

INTERNAL AUDITS

*Discuss Any Outstanding Issues (or Attach Summary):*

EXTERNAL AUDITS

*Discuss Any Outstanding Issues (or Attach Summary):*

**6. PT SAMPLES**

The following PT samples are now in house (Due Dates):

xx

**7. CERTIFICATIONS**

Certification Packages Being Worked On (Include Due Date):

x

Describe any issues, lapses, or potential revocations.

**8. REGULATORY UPDATE**

*Include information on new state or federal regulations that may impact the laboratory – new methods that require new instrumentation, deletion of methods, changes in sampling requirements or frequencies, ...*

**9. MISCELLANEOUS**

*Include any issues that may impact quality within the laboratory.*

**10. NEXT MONTH**

*Items planned for next month.*

LAB DIRECTOR COMMENTS AND PLANNED CORRECTIVE ACTIONS:	
LAB DIRECTOR REVIEW:	DATE:

**Figure 17-2.**

**Example - Laboratory Metrics Categories**

# Reports for month
# Reports revised due to lab error
<b>% Revised Reports</b>
<b># of Data Recall Investigations</b>
<b># of Reports Actually Recalled</b>
# Corrective Action Reports
# Corrective Action Reports still open
<b>Total Number of Unresolved Open Corrective Action Reports</b>
<b>% of Unresolved Open Corrective Action Reports</b>
# Reports independent QA reviewed
<b>% QA Data Review: Reports</b>
# Technical staff (Analysts/technicians, including Temps)
# of Analyst work product reviewed year-to-date
# of Analytical instruments w/electronic data file storage capability
# of Analytical instruments reviewed for data authenticity year-to-date
<b>% Analyst/Instrument Data Authenticity Audits</b>
<b># Client Complaints</b>
<b># Client Compliments</b>
# of planned internal audits
# of planned internal method audits performed year-to-date
<b>% Annual Internal Audits Complete</b>
<b># of Open Internal Audit Findings Past Due</b>
<b>Total Number of External Audit Findings</b>
<b># of Open External Audit Findings Past Due</b>
<b>% External Audit Findings Past Due</b>
# of PT analytes participated and received scores
# of PT analytes not acceptable
<b>% PT Cumulative Score</b>
<b># PT Repeat Analyte Failures Cumulative (analyte failed more than once in 4 consecutive studies by PT Type) (only applies to failed analytes)</b>
# SOPs

# SOPs Reviewed/ revised within 24 months
# Methods or Administrative procedures without approved SOPs
<b>SOP Status</b>
<b>Method certification Losses due to performance/audit issues</b>
<b>Hold Time Violations due to lab error</b>
<b>Date of Last Comprehensive Ethics Training Session</b>
<b># Staff that haven't Received Comprehensive Ethics Training (&gt;30 Days From Employment Date)</b>
<b>MDL Status (Good, Fair, or Poor) &gt;90%, &gt;70%, &lt;70%</b>
<b>Training Documentation Records (Good, Fair, or Poor)</b>
<b>LQM Revision/review Date</b>
<b>QAM Updated to New Integrated Template</b>
<b>Last Annual Internal Audit Date (Opened, Closed)</b>
<b>Last Management QS Review Date</b>
#SOPs required for 12 month review cycle (DOD or drinking water)
#SOPs for 12 month cycle/revised within 12 months (Includes QS and Methods Listed in QSM)
<b>12 month % SOP Status</b> (Includes QS and Methods Listed in QSM)

## **SECTION 18**

### **PERSONNEL (NELAC 5.5.2)**

#### **18.1 OVERVIEW**

TestAmerica's management believes that its highly qualified and professional staff is the single most important aspect in assuring a high level of data quality and service. The staff consists of professionals and support personnel as outlined in the organization chart in Appendix 2.

All personnel must demonstrate competence in the areas where they have responsibility. Any staff that is undergoing training shall have appropriate supervision until they have demonstrated their ability to perform their job function on their own. Staff shall be qualified for their tasks based on appropriate education, training, experience and/or demonstrated skills as required.

The laboratory employs sufficient personnel with the necessary education, training, technical knowledge and experience for their assigned responsibilities.

All personnel are responsible for complying with all QA/QC requirements that pertain to the laboratory and their area of responsibility. Each staff member must have a combination of experience and education to adequately demonstrate a specific knowledge of their particular area of responsibility. Technical staff must also have a general knowledge of lab operations, test methods, QA/QC procedures and records management.

Laboratory management is responsible for formulating goals for lab staff with respect to education, training and skills and ensuring that the laboratory has a policy and procedures for identifying training needs and providing training of personnel. The training shall be relevant to the present and anticipated responsibilities of the lab staff.

The laboratory only uses personnel that are employed by or under contract to, the laboratory. Contracted personnel, when used, must meet competency standards of the laboratory and work in accordance to the laboratory's quality system.

#### **18.2 EDUCATION AND EXPERIENCE REQUIREMENTS FOR TECHNICAL PERSONNEL**

TestAmerica makes every effort to hire analytical staff that possess a college degree (AA, BA, BS) in an applied science with some chemistry in the curriculum. Exceptions can be made based upon the individual's experience and ability to learn. There are competent analysts and technicians in the industry who have not earned a college degree. Selection of qualified candidates for laboratory employment begins with documentation of minimum education, training, and experience prerequisites needed to perform the prescribed task. Minimum education and training requirements for TestAmerica employees are outlined in job descriptions and are generally summarized for analytical staff in the table below.

The laboratory maintains job descriptions for all personnel who manage, perform or verify work affecting the quality of the environmental testing the laboratory performs. Job Descriptions are

located on the TestAmerica intranet site's Human Resources web-page (Also see Section 4 for position descriptions/responsibilities).

Experience and specialized training are occasionally accepted in lieu of a college degree (basic lab skills such as using a balance, colony counting, aseptic or quantitation techniques, etc. are also considered).

As a general rule for analytical staff:

Specialty	Education	Experience
Extractions, Digestions, some electrode methods (pH, DO, Redox, etc.), or Titrimetric and Gravimetric Analyses	H.S. Diploma	On the job training (OJT)
GFAA, CVAA, FLAA, Single component or short list Chromatography (e.g., Fuels, BTEX-GC, IC	A college degree in an applied science or 2 years of college and at least 1 year of college chemistry	Or 2 years prior analytical experience is required
ICP, ICPMS, Long List or complex chromatography (e.g., Pesticides, PCB, Herbicides, HPLC, etc.), GCMS	A college degree in an applied science or 2 years of college chemistry	or 5 years of prior analytical experience
Spectra Interpretation	A college degree in an applied science or 2 years of college chemistry	And 2 years relevant experience Or 5 years of prior analytical experience
Technical Directors/Department Managers – <b><u>General</u></b>	Bachelors Degree in an applied science or engineering with 24 semester hours in chemistry  An advanced (MS, PhD.) degree may substitute for one year of experience	And 2 years experience in environmental analysis of representative analytes for which they will oversee

When an analyst does not meet these requirements, they can perform a task under the direct supervision of a qualified analyst, peer reviewer or Department Manager, and are considered an analyst in training. The person supervising an analyst in training is accountable for the quality of the analytical data and must review and approve data and associated corrective actions.

### 18.3 **TRAINING**

TestAmerica is committed to furthering the professional and technical development of employees at all levels.

Orientation to the laboratory’s policies and procedures, in-house method training, and employee attendance at outside training courses and conferences all contribute toward employee proficiency. Below are examples of various areas of required employee training:

Required Training	Time Frame*	Employee Type
Environmental Health & Safety	Refer to EH&S Manual	All
Ethics – New Hires	1 week of hire	All
Ethics - Comprehensive	90 days of hire	All
Data Integrity	30 days of hire	Technical and PMs
Quality Assurance	90 days of hire	All
Ethics – Comprehensive Refresher	Annually	All
Initial Demonstration of Capability (DOC)	Prior to unsupervised method performance	Technical

The laboratory maintains records of relevant authorization/competence, education, professional qualifications, training, skills and experience of technical personnel (including contracted personnel) as well as the date that approval/authorization was given. These records are kept on file at the laboratory. Also refer to “Demonstration of Capability” in Section 20.

The training of technical staff is kept up to date by:

- Each employee must have documentation in their training file that they have read, understood and agreed to follow the most recent version of the laboratory QA Manual and SOPs in their area of responsibility. This documentation is updated as SOPs are updated.
- Documentation from any training courses or workshops on specific equipment, analytical techniques or other relevant topics are maintained in their training file.
- Documentation of proficiency (refer to Section 20).
- An Ethics Agreement signed by each staff member (renewed each year) and evidence of annual ethics training.
- A Confidentiality Agreement signed by each staff member signed at the time of employment.
- Human Resources maintains documentation and attestation forms on employment status & records; benefit programs; timekeeping/payroll; and employee conduct (e.g., ethics). This information is maintained in the employee’s secured personnel file.

Further details of the laboratory's training program are described in the Laboratory Training SOP SAC-QA-0022, “Employee Orientation and Training”.

#### **18.4 DATA INTEGRITY AND ETHICS TRAINING PROGRAM**

Establishing and maintaining a high ethical standard is an important element of a Quality System. Ethics and data integrity training is integral to the success of TestAmerica and is provided for each employee at TestAmerica. It is a formal part of the initial employee orientation within 1 week of hire, comprehensive training within 90 days, and an annual refresher for all employees. Senior management at each facility performs the ethics training for their staff.

In order to ensure that all personnel understand the importance TestAmerica places on maintaining high ethical standards at all times; TestAmerica has established an Ethics Policy No. CA-L-P-001 and an Ethics Statement/Agreement (Appendix 1). All initial and annual training is documented by signature on the signed Ethics Policy and Code of Ethical Conduct demonstrating that the employee has participated in the training and understands their obligations related to ethical behavior and data integrity.

Violations of this Ethics Policy will not be tolerated. Employees who violate this policy will be subject to disciplinary actions up to and including termination. Criminal violations may also be referred to the Government for prosecution. In addition, such actions could jeopardize TestAmerica's ability to do work on Government contracts, and for that reason, TestAmerica has a Zero Tolerance approach to such violations.

Employees are trained as to the legal and environmental repercussions that result from data misrepresentation. Key topics covered in the presentation include:

- Organizational mission and its relationship to the critical need for honesty and full disclosure in all analytical reporting.
- Ethics Policy (Appendix 1)
- How and when to report ethical/data integrity issues. Confidential reporting.
- Record keeping.
- Discussion regarding data integrity procedures.
- Specific examples of breaches of ethical behavior (e.g. peak shaving, altering data or computer clocks, improper macros, etc., accepting/offering kickbacks, illegal accounting practices, unfair competition/collusion)
- Internal monitoring. Investigations and data recalls.
- Consequences for infractions including potential for immediate termination, debarment, or criminal prosecution.
- Importance of proper written narration / data qualification by the analyst and project manager with respect to those cases where the data may still be usable but are in one sense or another partially deficient.

Additionally, a data integrity hotline (1-800-736-9407) is maintained by TestAmerica and administered by the Corporate Quality Department.

## SECTION 19

### ACCOMMODATIONS AND ENVIRONMENTAL CONDITIONS (NELAC 5.5.3)

#### 19.1 OVERVIEW

TestAmerica West Sacramento is a 66,000 ft<sup>2</sup> secure laboratory facility with controlled access and designed to accommodate an efficient workflow and to provide a safe and comfortable work environment for employees. All visitors sign in and are escorted by laboratory personnel. Access is controlled by various measures.

The laboratory is equipped with structural safety features. Each employee is familiar with the location, use, and capabilities of general and specialized safety features associated with their workplace. The laboratory provides and requires the use of protective equipment including safety glasses, protective clothing, gloves, etc. OSHA and other regulatory agency guidelines regarding required amounts of bench and fume hood space, lighting, ventilation (temperature and humidity controlled), access, and safety equipment are met or exceeded.

Traffic flow through sample preparation and analysis areas is minimized to reduce the likelihood of contamination. Adequate floor space and bench top area is provided to allow unencumbered sample preparation and analysis space. Sufficient space is also provided for storage of reagents and media, glassware, and portable equipment. Ample space is also provided for refrigerated sample storage before analysis and archival storage of samples after analysis. Laboratory HVAC and deionized water systems are designed to minimize potential trace contaminants.

The laboratory is separated into specific areas for sample receiving, sample preparation, volatile organic sample analysis, non-volatile organic sample analysis, inorganic sample analysis, and administrative functions.

#### 19.2 ENVIRONMENT

Laboratory accommodation, test areas, energy sources, lighting are adequate to facilitate proper performance of tests. The facility is equipped with heating, ventilation, and air conditioning (HVAC) systems appropriate to the needs of environmental testing performed at this laboratory.

The environment in which these activities are undertaken does not invalidate the results or adversely affect the required accuracy of any measurements.

The laboratory provides for the effective monitoring, control and recording of environmental conditions that may affect the results of environmental tests as required by the relevant specifications, methods, and procedures. Such environmental conditions include humidity, voltage, and temperature in the laboratory. In the event of a power outage, the laboratory can be equipped with a back up power supply for sample storage, as detailed in SOP No. SAC-QA-0005, "Temperature Monitoring and Corrective Action for Refrigerators and Freezers".

When any of the method or regulatory required environmental conditions change to a point where they may adversely affect test results, analytical testing will be discontinued until the environmental conditions are returned to the required levels (refer to Section 12).

Environmental conditions of the facility housing the computer network and LIMS are regulated to protect against raw data loss.

### **19.3 WORK AREAS**

There is effective separation between neighboring areas when the activities therein are incompatible with each other. Examples include:

- Volatile organic chemical handling areas, including sample preparation and waste disposal, and volatile organic chemical analysis areas.

Access to and use of all areas affecting the quality of analytical testing is defined and controlled by secure access to the laboratory building as described below in the Building Security section.

Adequate measures are taken to ensure good housekeeping in the laboratory and to ensure that any contamination does not adversely affect data quality. These measures include regular cleaning to control dirt and dust within the laboratory.

Work areas are available to ensure an unencumbered work area. Work areas include:

- Access and entryways to the laboratory.
- Sample receipt areas.
- Sample storage areas.
- Chemical and waste storage areas.
- Data handling and storage areas.
- Sample processing areas.
- Sample analysis areas.

### **19.4 FLOOR PLAN**

A floor plan can be found in Appendix 3.

**19.5      BUILDING SECURITY**

Building keys and alarm codes are distributed to employees as necessary.

Employees wear photographic identification name cards while on the premises.

Visitors to the laboratory sign in and out in a visitor's logbook. A visitor is defined as any person who visits the laboratory who is not an employee of TestAmerica West Sacramento. In addition to signing into the laboratory, the Environmental, Health and Safety Manual contains requirements for visitors and vendors. There are specific safety forms that must be reviewed and signed.

Visitors (with the exception of company employees) are escorted by laboratory personnel at all times, or the location of the visitor is noted in the visitor's logbook.

## SECTION 20.0

### TEST METHODS AND METHOD VALIDATION (NELAC 5.5.4)

#### 20.1 OVERVIEW

TestAmerica West Sacramento uses methods that are appropriate to meet our clients' requirements and that are within the scope of the laboratory's capabilities. These include sampling, handling, transport, storage and preparation of samples, and, where appropriate, an estimation of the measurement of uncertainty as well as statistical techniques for analysis of environmental data.

Instructions are available in the laboratory for the operation of equipment as well as for the handling and preparation of samples. All instructions, Standard Operating Procedures (SOPs), reference methods and manuals relevant to the working of the laboratory are readily available to all staff. Deviations from published methods are documented (with justification) in the laboratory's approved SOPs. SOPs are submitted to clients for review at their request. Significant deviations from published methods require client approval and regulatory approval where applicable.

#### 20.2 STANDARD OPERATING PROCEDURES (SOPs)

TestAmerica West Sacramento maintains SOPs that accurately reflect all phases of the laboratory such as assessing data integrity, corrective actions, handling customer complaints as well as all analytical methods and sampling procedures. The method SOPs are derived from the most recently promulgated/approved, published methods and are specifically adapted to the laboratory facility. Modifications or clarifications to published methods are clearly noted in the SOPs. All SOPs are controlled in the laboratory (refer to Section 6 on Document Control):

- All SOPs contain a revision number, effective date, and appropriate approval signatures. Controlled copies are available to all staff.
- Procedures for preparation, review, revision and control are incorporated by reference to SOPs: CW-Q-S-002 (Writing a Standard Operating Procedure (SOP) and WS-QA-0021 (Preparation and Management of Standard Operating Procedures).
- SOPs are reviewed at a minimum of every 2 years (annually for Drinking Water and DoD SOPs), and where necessary, revised to ensure continuing suitability and compliance with applicable requirements.

#### 20.3 LABORATORY METHODS MANUAL

For each test method, the laboratory shall have available the published referenced method as well as the laboratory developed SOP. Refer to the corporate SOP CW-Q-S-002 "Writing a Standard Operating Procedure" for content and requirements of technical and non-technical SOPs, as well as SOP WS-QA-0021, "Preparation and Management of Standard Operating Procedures".

**Note:** If more stringent standards or requirements are included in a mandated test method or regulation than those specified in this manual, the laboratory shall demonstrate that such

requirements are met. If it is not clear which requirements are more stringent, the standard from the method or regulation is to be followed. Any exceptions or deviations from the referenced methods or regulations are noted in the specific analytical SOP.

## **20.4 SELECTION OF METHODS**

Since numerous methods and analytical techniques are available, continued communication between the client and laboratory is imperative to assure the correct methods are utilized. Once client methodology requirements are established, this and other pertinent information is summarized by the Project Manager. These mechanisms ensure that the proper analytical methods are applied when the samples arrive for log-in. For non-routine analytical services (e.g., special matrices, non-routine compound lists, etc.), the method of choice is selected based on client needs and available technology. The methods selected should be capable of measuring the specific parameter of interest, in the concentration range of interest, and with the required precision and accuracy.

### **20.4.1 Sources of Methods**

Routine analytical services are performed using standard EPA-approved methodology. In some cases, modification of standard approved methods may be necessary to provide accurate analyses of particularly complex matrices. When the use of specific methods for sample analysis is mandated through project or regulatory requirements, only those methods shall be used.

In general, TestAmerica West Sacramento follows procedures from the referenced methods shown below in 20.4.1.1.

When clients do not specify the method to be used or methods are not required, the methods used will be clearly validated and documented in an SOP and available to clients and/or the end user of the data.

**20.4.1.1** The analytical methods used by the laboratory are those currently accepted and approved by the U. S. EPA and the state or territory from which the samples were collected. Reference methods include:

- Method 1664, Revision A: N-Hexane Extractable Material (HEM; Oil and Grease) and Silica Gel Treated N-Hexane Extractable Material (SGT-HEM); Non-polar Material) by Extraction and Gravimetry, EPA-821-R-98-002, February 1999
- Compendium of Methods for the Determination of Toxic Organic Compounds in Ambient Air, US EPA, January 1996.
- Guidelines Establishing Test Procedures for the Analysis of Pollutants Under the Clean Water Act, and Appendix A-C; 40 CFR Part 136, USEPA Office of Water. Revised as of July 1, 1995, Appendix A to Part 136 - Methods for Organic Chemical Analysis of Municipal and Industrial Wastewater (EPA 600 Series)
- Methods for Chemical Analysis of Water and Wastes, EPA 600 (4-79-020), 1983.
- Methods for the Determination of Inorganic Substances in Environmental Samples, EPA-600/R-93/100, August 1993.

- Methods for the Determination of Metals in Environmental Samples, EPA/600/4-91/010, June 1991. Supplement I: EPA-600/R-94/111, May 1994.
- Methods for the Determination of Organic Compounds in Drinking Water, EPA-600/4-88-039, December 1988, Revised, July 1991, Supplement I, EPA-600-4-90-020, July 1990, Supplement II, EPA-600/R-92-129, August 1992. Supplement III EPA/600/R-95/131 - August 1995 (EPA 500 Series) (EPA 500 Series methods)
- Technical Notes on Drinking Water Methods, EPA-600/R94-173, October 1994
- Statement of Work for Inorganics Analysis, ILM04.1, USEPA Contract Laboratory Program Multi-media, Multi-concentration.
- Statement of Work for Organics Analysis, OLM04.2, USEPA Contract Laboratory Program, Multi-media, Multi-concentration.
- Statement of Work for Organic Analysis, Multi-Media, Multi-Concentration, OLMO4.1, USEPA Contract Laboratory Program, September 1998.
- Standard Methods for the Examination of Water and Wastewater, 18<sup>th</sup>/19<sup>th</sup>/20<sup>th</sup>/21<sup>st</sup> edition; Eaton, A.D. Clesceri, L.S. Greenberg, A.E. Eds; American Water Works Association, Water Pollution Control Federation, American Public Health Association: Washington, D.C.
- Test Methods for Evaluating Solid Waste Physical/Chemical Methods (SW846), Third Edition, September 1986, Final Update I, July 1992, Final Update IIA, August 1993, Final Update II, September 1994; Final Update IIB, January 1995; Final Update III, December 1996.
- Annual Book of ASTM Standards, American Society for Testing & Materials (ASTM), Philadelphia, PA.
- National Status and Trends Program, National Oceanographic and Atmospheric Administration, Volume I-IV, 1985-1994.
- Manual for the Certification of Laboratories Analyzing Drinking Water, (EPA 815-R-05-004, January 2005)
- Code of Federal Regulations (CFR) 40, Parts 136, 141, 172, 173, 178, 179 and 261
- Underground Storage Tanks Procedures Manual, State of Alaska Department of Environmental Conservation, Division of Spill Prevention and Response Contaminated Sites Program, November 7, 2002
- Leaking Underground Fuel Tank Field Manual: Guidelines for Site Assessment, Cleanup, and Underground Storage Tank Closure, State of California Leaking Underground Fuel Tank Task Force, October, 1989
- Tri-Regional Board Staff Recommendations for Preliminary Investigation and Evaluation of Underground Tank Sites, North Coast Regional Water Quality Control Board, San Francisco Bay Regional Water Quality Control Board and Central Valley Regional Water Quality Control Board, August 10, 1990
- Analytical Methods for Petroleum Hydrocarbons, Washington State Department of Ecology, June 1997
- Compendium of Methods for the Determination of Air Pollutants in Indoor Air, (EPA 600/4-90-10, April 1990)
- Compendium of Methods for the Determination of Inorganic Compounds in Ambient Air, (EPA 625/R-96/010a, June 1999)
- Methods for Determining Emissions of Toxic Air Contaminants from Stationary Sources, Stationary Source Test Methods, Volume 3, California Air Resources Board

The laboratory reviews updated versions to all the aforementioned references for adaptation based upon capabilities, instrumentation, etc., and implements them as appropriate. As such, the laboratory strives to perform only the latest versions of each approved method as regulations allow or require.

Other reference procedures for non-routine analyses may include methods established by specific states (e.g., Underground Storage Tank methods), ASTM or equipment manufacturers. Sample type, source, and the governing regulatory agency requiring the analysis will determine the method utilized.

The laboratory shall inform the client when a method proposed by the client may be inappropriate or out of date. After the client has been informed, and they wish to proceed contrary to the laboratory's recommendation, it will be documented.

#### **20.4.2 Demonstration of Capability**

Before the laboratory may institute a new method and begin reporting results, the laboratory shall confirm that it can properly operate the method. In general, this demonstration does not test the performance of the method in real world samples, but in an applicable and available clean matrix sample. If the method is for the testing of analytes that are not conducive to spiking, demonstration of capability may be performed on quality control samples.

**20.4.2.1** A demonstration of capability is performed whenever there is a change in instrument type, method or personnel.

**20.4.2.2** The initial demonstration of capability must be thoroughly documented and approved by the Technical Director and QA Manager prior to independently analyzing client samples. All associated documentation must be retained in accordance with the laboratories archiving procedures (refer to Section 15, Control of Records).

**20.4.2.3** The laboratory must have an approved SOP, demonstrate satisfactory performance, and conduct a method detection limit study (when applicable). There may be other requirements as stated within the published method or regulations (i.e., retention time window study).

**Note:** In some instances, a situation may arise where a client requests that an unusual analyte be reported using a method where this analyte is not normally reported. If the analyte is being reported for regulatory purposes, the method must meet all procedures outlined within this QA Manual (SOP, MDL, and Demonstration of Capability). If the client states that the information is not for regulatory purposes, the result may be reported as long as the following criteria are met:

- The instrument is calibrated for the analyte to be reported using the criteria for the method and ICV/CCV criteria are met (unless an ICV/CCV is not required by the method).
- The reporting limit is set at or above the first standard of the curve for the analyte.

- The client request is documented and the lab informs the client of its procedure for working with unusual compounds. The final report must be footnoted: *Reporting Limit based on the low standard of the calibration curve.*
- Refer to Section 12 (Control of Non-Conforming Work).

### **20.4.3 Initial Demonstration of Capability (IDOC) Procedures**

**20.4.3.1** The spiking standard used must be prepared independently from those used in instrument calibration.

**20.4.3.2** The analyte(s) shall be diluted in a volume of clean matrix sufficient to prepare four aliquots at the concentration specified by a method or the laboratory SOP.

**20.4.3.3** At least four aliquots shall be prepared (including any applicable clean-up procedures) and analyzed according to the test method (either concurrently or over a period of days).

**20.4.3.4** Using all of the results, calculate the mean recovery in the appropriate reporting units and the standard deviations for each parameter of interest.

**20.4.3.5** When it is not possible to determine the mean and standard deviations, such as for presence, absence and logarithmic values, the laboratory will assess performance against criteria described in the Method SOP.

**20.4.3.6** Compare the information obtained above to the corresponding acceptance criteria for precision and accuracy in the test method (if applicable) or in laboratory generated acceptance criteria (LCS or interim criteria) if there is no mandatory criteria established. If any one of the parameters do not meet the acceptance criteria, the performance is unacceptable for that parameter.

**20.4.3.7** When one or more of the tested parameters fail at least one of the acceptance criteria, the analyst must proceed according to either option listed below:

- Locate and correct the source of the problem and repeat the test for all parameters of interest beginning with 20.4.3.3 above.
- Beginning with 20.4.3.3 above, repeat the test for all parameters that failed to meet criteria. Repeated failure, however, will confirm a general problem with the measurement system. If this occurs, locate and correct the source of the problem and repeat the test for all compounds of interest beginning with 20.4.3.1 above.

A certification statement (see Figure 20-1 as an example) shall be used to document the completion of each initial demonstration of capability. A copy of the certification is archived in the analyst's training folder.

## **20.5 LABORATORY DEVELOPED METHODS AND NON-STANDARD METHODS**

Any new method developed by the laboratory must be fully defined in an SOP/Methods Manual (Section 20.2) and validated by qualified personnel with adequate resources to perform the method. Method specifications and the relation to client requirements must be clearly conveyed to the client if the method is a non-standard method (not a published or routinely accepted method). The client must also be in agreement to the use of the non-standard method. The information included in the checklist below (Figure 20-2) is needed before samples are accepted for analysis by a new method.

## **20.6 VALIDATION OF METHODS**

Validation is the confirmation by examination and the provision of objective evidence that the particular requirements for a specific intended use are fulfilled. (From 2003 NELAC Standard)

All non-standard methods, laboratory designed/developed methods, standard methods used outside of their scope, and major modifications to published methods must be validated to confirm they are fit for their intended use. The validation will be as extensive as necessary to meet the needs of the given application. The results are documented with the validation procedure used and contain a statement as to the fitness for use.

### **20.6.1 Method Validation and Verification Activities for All New Methods**

While method validation can take various courses, the following activities can be required as part of method validation. Method validation records are designated QC records and are archived accordingly.

#### **20.6.1.1 Determination of Method Selectivity**

Method selectivity is the demonstrated ability to discriminate the analyte(s) of interest from other compounds in the specific matrix or matrices from other analytes or interference. In some cases to achieve the required selectivity for an analyte, a confirmation analysis is required as part of the method.

#### **20.6.1.2 Determination of Method Sensitivity**

Sensitivity can be both estimated and demonstrated. Whether a study is required to estimate sensitivity depends on the level of method development required when applying a particular measurement system to a specific set of samples. Where estimations and/or demonstrations of sensitivity are required by regulation or client agreement, such as the procedure in 40 CFR Part 136 Appendix B, under the Clean Water Act, these shall be followed. The laboratory determinations of MDLs are described in Section 20.7.

#### **20.6.1.3 Relationship of Limit of Detection (LOD) to the Quantitation Limit (QL)**

An important characteristic of expression of sensitivity is the difference in the LOD and the QL. The LOD is the minimum level at which the presence of an analyte can be reliably concluded. The QL is the minimum level at which both the presence of an analyte and its concentration can be reliably determined. For most instrumental measurement systems, there is a region where semi-quantitative data is generated around the LOD (both above and below the estimated MDL or LOD) and below the QL. In this region, detection of an analyte may be confirmed but quantification of the analyte is unreliable within the accuracy and precision guidelines of the

measurement system. When an analyte is detected below the QL, and the presence of the analyte is confirmed by meeting the qualitative identification criteria for the analyte, the analyte can be reliably reported, but the amount of the analyte can only be estimated. If data is to be reported in this region, it must be done so with a qualification that denotes the semi-quantitative nature of the result.

#### **20.6.1.4 Determination of Interferences**

A determination that the method is free from interferences in a blank matrix is performed.

#### **20.6.1.5 Determination of Range**

Where appropriate, a determination of the applicable range of the method may be performed. In most cases, range is determined and demonstrated by comparison of the response of an analyte in a curve to established or targeted criteria. The curve is used to establish the range of quantitation and the lower and upper values of the curve represent upper and lower quantitation limits. Curves are not limited to linear relationships.

#### **20.6.1.6 Determination of Accuracy and Precision**

Accuracy and precision studies are generally performed using replicate analyses, with a resulting percent recovery and measure of reproducibility (standard deviation, relative standard deviation) calculated and measured against a set of target criteria.

#### **20.6.1.7 Documentation of Method**

The method is formally documented in an SOP. If the method is a minor modification of a standard laboratory method that is already documented in an SOP, an SOP Attachment describing the specific differences in the new method is acceptable in place of a separate SOP.

#### **20.6.1.8 Continued Demonstration of Method Performance**

Continued demonstration of Method Performance is addressed in the SOP. Continued demonstration of method performance is generally accomplished by batch specific QC samples such as LCS, method blanks or PT samples.

### **20.7 METHOD DETECTION LIMITS (MDL)/ LIMITS OF DETECTION (LOD)**

Method detection limits (MDL) are initially determined in accordance with 40 CFR Part 136, Appendix B or alternatively by other technically acceptable practices that have been accepted by regulators. MDL is also sometimes referred to as Limit of Detection (LOD). The MDL theoretically represents the concentration level for each analyte within a method at which the Analyst is 99% confident that the true value is not zero. The MDL is determined for each analyte initially during the method validation process and updated as required in the analytical methods, whenever there is a significant change in the procedure or equipment, or based on project specific requirements (refer to 20.7.10). The analyst prepares at least seven replicates of solution spiked at one to five times the estimated method detection limit (most often at the lowest standard in the calibration curve) into the applicable matrix with all the analytes of interest. Each of these aliquots is extracted (including any applicable clean-up procedures) and analyzed in the same manner as

the samples. Where possible, the seven replicates should be analyzed over 2-4 days to provide a more realistic MDL. Alternatively, the MDL may be determined using a series (ideally 50-100) method blanks for “uncensored” methods which always return a signal (i.e., ICP). See SOP SAC-QA-0006, “Method Detection Limits (MDL) and Instrument Detection Limits (IDL)”, for specifics.

**20.7.1** MDL’s are initially performed for each individual instrument and non-microbiological method analysis. Unless there are requirements to the contrary, the laboratory will use the highest calculated MDL for all instruments used for a given method as the MDL for reporting purposes. This MDL is not required for methods that are not readily spiked (e.g. pH, turbidity, etc.) Titration and gravimetric methods where there is no additional preparation involved, the MDL is based on the lowest discernable unit of measure that can be observed.

**20.7.2** MDL’s must be run against acceptable instrument QC, including ICV’s and Tunes. This is to insure that the instrument is in proper working condition and falsely high or low MDL’s are not calculated.

**20.7.3** Use only clean matrix which is free of target analytes (e.g.: Laboratory reagent water, Ottawa Sand) unless a project specific MDL is required in a field sample matrix.

**20.7.4** The Reporting Limit (also may be referred to as Limit of Quantitation or LOQ) should generally be between 2 and 5 times the MDL. If the MDL is being performed during method development, use this guideline to determine the Reporting Limit for the analysis, e.g., the DoD QSM requires that the RL is  $\geq 3x$  MDL. If a sample is diluted, the reported MDL is adjusted according to the dilution factor.

**20.7.5** The calculated MDL cannot be greater than the spike amount.

**20.7.6** If the most recent calculated MDL does not permit qualitative identification of the analyte then the laboratory may use technical judgment for establishing the MDL (e.g., calculate what level would give a qualitative ID, compare with IDL (20.7), spike at a level where qualitative ID is determined and assign that value as MDL, minimum sensitivity requirements, Standard deviation of method blanks over time, etc.). These alternate verification procedures must be documented in the laboratory SOP on MDL’s. See SOP SAC-QA-0006, “Method Detection Limits (MDL) and Instrument Detection Limits (IDL)” for further details of the procedures.

**20.7.7** Each of the 7 spikes must be qualitatively identifiable (e.g., appear in both columns for dual column methods, characteristic ions for GCMS mass spectra, etc). Manual integrations to force the baseline for detection are not allowed.

**20.7.8** The initial MDL is calculated as follows:

$$\text{MDL} = t_{(n-1, 1-a = 0.99)} \times (\text{Standard Deviation of replicates})$$

where  $t_{(n-1, 1-a = 0.99)} = 3.143$  for seven replicates.

**20.7.9** Subsequent to the initial MDL determination, periodic MDL verification, confirmation or determinations may be performed by the procedure in 40 CFR Part 136, Appendix B or alternatively by other technically acceptable practices (e.g., method blanks over time, single

standard spikes that have been subjected to applicable sample prep processes, etc.). The procedures utilized must be documented in the MDL SOP. See SOP SAC-QA-0006, "Method Detection Limits (MDL) and Instrument Detection Limits (IDL)" for further details of the procedures.

**20.7.10** Because of the inherent variability in results outside of the calibration range, TestAmerica does not recommend the reporting of results below the lowest calibration point in a curve; however, it is recognized that some projects and agencies require the reporting of results below the RL. Any result that falls between the MDL and the Reporting limit, when reported, will be qualified as an estimated value.

**20.7.11** Detections reported down to the MDL must be qualitatively identified.

**20.7.12** MDLs and Reporting limits are adjusted in LIMs based on moisture content and sample aliquot size.

## **20.8 INSTRUMENT DETECTION LIMITS (IDL)**

**20.8.1** The IDL is sometimes used to assess the reasonableness of the MDLs or in some cases required by the analytical method or program requirements. IDLs are most used in metals analyses but may be useful in demonstration of instrument performance in other areas.

**20.8.2** IDLs are calculated to determine an instrument's sensitivity independent of any preparation method. IDLs are calculated either using 7 replicate spike analyses, like MDL but without sample preparation, or by the analysis of 10 instrument blanks and calculating 3 x the absolute value of the standard deviation.

**20.8.3** If IDL is > than the MDL, it may be used as the reported MDL.

## **20.9 VERIFICATION OF DETECTION AND REPORTING LIMITS**

**20.9.1** Once an MDL is established, it must be verified, on each instrument, by analyzing a quality control sample (prepared as a sample) at approximately 2-3 times the calculated MDL. The analytes must be qualitatively identified or see section 20.7.7 for other options. This verification does not apply to methods that are not readily spiked (e.g. pH, turbidity, etc.) or where the lab does not report to the MDL. If the MDL does not verify, then the lab will not report to the MDL, or redevelop their MDL or use the level where qualitative identification is established (See 20.6.7). MDLs must be verified at least annually.

**20.9.2** When a Reporting limit is established, it must be initially verified by the analysis of a low level standard and annually thereafter. Unless there are requirements to the contrary the acceptance criteria is  $\pm 50\%$ . The annual requirement is waved for methods that have an annually verified MDL.

## **20.10 RETENTION TIME WINDOWS**

Most organic analyses and some inorganic analyses use chromatography techniques for qualitative and quantitative determinations. For every chromatography analysis each analyte will

have a specific time of elution from the column to the detector. This is known as the analyte's retention time. The variance in the expected time of elution is defined as the retention time window. As the key to analyte identification in chromatography, retention time windows must be established on every column for every analyte used for that method. These records are kept with the files associated with an instrument for later quantitation of the analytes.

For GC, HPLC and IC methods, there must be sufficient separation between analyte peaks so as to not misidentify analytes. In the mid-level standard, the distance between the valley and peak height cannot be any less than 25% of the sum of the peak heights of the analytes. This also applies to GCMS in the case where the two compounds share the same quantitation ion.

**Note:** Some analytes do not separate sufficiently to be able to identify or quantitate them as separate analytes (e.g. m-xylene and p-xylene) and are quantitated and reported as a single analyte (e.g. m,p-xylenes).

Once the analyst has determined that the instrument is in optimum working condition through calibration and calibration verification procedures, he or she uses a mid-range calibration or calibration verification standard to establish the retention times for each of the individual analytes in a method. The analyst makes three injections of the same standard over a 72-hour (24 hr period for 300.0) period, tabulating the retention times for each analyte for each of the three injections. The width of the retention time window is normally the average absolute retention time  $\pm$  3 Standard Deviations. A peak outside the retention time window will not be identified by the computer as a positive match of the analyte of interest.

It is possible for the statistically calculated RT window to be too tight and need to be adjusted based on analyst experience. In these instances method default retention time windows may be used (e.g., for 8000 series methods a default of 0.03 minutes may be used, and EPA CLP 0.05 minutes is used). The same concept is applied when any peak outside of that window will not be identified by the computer as a positive match.

The calibration verification standard at the beginning of a run may be used to adjust the RT for an analyte. This is essentially re-centering the window but the size of the window remains the same. The RTs are verified when all analytes are within their RT windows and are properly identified.

## **20.11 EVALUATION OF SELECTIVITY**

The laboratory evaluates selectivity by following the checks within the applicable analytical methods, which include mass spectral tuning, second column confirmation, ICP interelement interference checks, chromatography retention time windows, sample blanks, spectrochemical, atomic absorption or fluorescence profiles, co-precipitation evaluations and specific electrode response factors.

## **20.12 ESTIMATION OF UNCERTAINTY OF MEASUREMENT**

**20.12.1** Uncertainty is "a parameter associated with the result of a measurement, that characterizes the dispersion of the values that could reasonably be attributed to the measurand" (as defined by the International Vocabulary of Basic and General Terms in Metrology, ISO Geneva, 1993, ISBN 92-67-10175-1). Knowledge of the uncertainty of a measurement provides additional confidence in a result's validity. Its value accounts for all the factors which could

possibly affect the result, such as adequacy of analyte definition, sampling, matrix effects and interferences, climatic conditions, variances in weights, volumes, and standards, analytical procedure, and random variation. Some national accreditation organizations require the use of an “expanded uncertainty”: the range within which the value of the measurand is believed to lie within at least a 95% confidence level with the coverage factor  $k=2$ .

**20.12.2** Uncertainty is not error. Error is a single value, the difference between the true result and the measured result. On environmental samples, the true result is never known. The measurement is the sum of the unknown true value and the unknown error. Unknown error is a combination of systematic error, or bias, and random error. Bias varies predictably, constantly, and independently from the number of measurements. Random error is unpredictable, assumed to be Gaussian in distribution, and reducible by increasing the number of measurements.

**20.12.3** The uncertainty associated with results generated by the laboratory can be determined by using the Laboratory Control Sample (LCS) accuracy range for a given analyte. The LCS limits are used to assess the performance of the measurement system since they take into consideration all of the laboratory variables associated with a given test over time (except for variability associated with the sampling). The percent recovery of the LCS is compared either to the method-required LCS accuracy limits or to the statistical, historical, in-house LCS accuracy limits.

**20.12.4** To calculate the uncertainty for the specific result reported, multiply the result by the decimal of the lower end of the LCS range percent value for the lower end of the uncertainty range, and multiply the result by the decimal of the upper end of the LCS range percent value for the upper end of the uncertainty range. These calculated values represent a 99%-certain range for the reported result. As an example, suppose that the result reported is 1.0 mg/l, and the LCS percent recovery range is 50 to 150%. The uncertainty range would be 0.5 to 1.5 mg/l, which could also be written as 1.0 +/- 0.5 mg/l.

**20.12.5** In the case where a well recognized test method specifies limits to the values of major sources of uncertainty of measurement (e.g. 524.2, 525, etc) and specifies the form of presentation of calculated results, no further discussion of uncertainty is required.

## **20.13**      **CONTROL OF DATA**

The laboratory has policies and procedures in place to ensure the authenticity, integrity, and accuracy of the analytical data generated by the laboratory.

### **20.13.1**      **Computer and Electronic Data Related Requirements**

The three basic objectives of our computer security procedures and policies are shown below. More detail is outlined in SOP Nos. S-ITQ-005, “QuantIMS/JDE user Profile Setup and Maintenance”, and S-ITQ-007, “Software Testing, Validation and Verification. The laboratory is currently running QuantIMS which is a custom in-house developed LIMS system that has been highly customized to meet the needs of the laboratory. It is referred to as LIMS for the remainder of this section. The LIMS utilizes DB2 which is an industry standard relational database platform. It is referred to as Database for the remainder of this section.

**20.13.1.1 Maintain the Database Integrity:** Assurance that data is reliable and accurate through data verification (review) procedures, password-protecting access, anti-virus protection, data change requirements, as well as an internal LIMS permissions procedure.

- LIMS Database Integrity is achieved through data input validation, internal user controls, and data change requirements.
- Spreadsheets and other software developed in-house must be verified with documentation through hand calculations prior to use.

**Note:** “Commercial off-the-shelf software in use within the designed application range is considered to be sufficiently validated.” *From NELAC 2003 Standard.* However, laboratory specific configurations or modifications are validated prior to use.

- In order to assure accuracy, all data entered or transferred into the LIMS data system goes through a minimum of two levels of review.
- The QA department performs random data audits to ensure the correct information has been reported.
- Changes to reports are documented in a spreadsheet.
- Analytical data file security is provided through three policies.
  - The first policy forbids unauthorized personnel from using laboratory data acquisition computers.
  - The second policy is the implementation of network passwords and login names that restrict directory access.
  - The third layer is maintained through the LIMS and includes the use of username/password combinations to gain access to the LIMS system, the fact that all data in the LIMS is associated with the user who added/reviewed the data, and the restriction of review authority of data.
- All software installations will be in accordance with any relevant copyright licensing regulations.
- All software installed on any computer within the laboratory must be approved by the Information Technology Department regional support technician assigned to the laboratory. Shrink-wrapped or otherwise sealed OEM software that is directly related to instrument usage does not need approval but the Information Technology department must be notified of the installation.
- Anti-virus software shall be installed on all servers and workstations. The anti-virus software shall be configured to check for virus signature file and program updates on a daily basis and these updates will be pushed to all servers and workstations. The anti-virus software will be configured to clean any virus-infected file if possible, otherwise the file will be deleted. Disks and CDs brought from any outside source that are not OEM software must be scanned for viruses before being accessed.
- **Interlab LIMS Permissions Policy**
  - PURPOSE - The purpose of this policy is to provide a mechanism for maintaining the integrity of information contained in each laboratory’s LIMS while providing the necessary access for information sharing to staff at other laboratory facilities.

- DEFINITIONS - Host Laboratory: The laboratory facility that 'owns' the LIMS system or 'hosts' a project/job.
- POLICIES
  - (a) All permissions for the laboratory's LIMS system must only be granted by a representative of that laboratory.
    - If someone outside of the host lab needs permissions for Project Management or other uses, they must go through the Lab Director or his/her designated representative.
    - Permissions must never be granted without the knowledge of the host laboratory.
  - (b) Only laboratory analytical or QA staff from the home laboratory may have edit permissions for laboratory analysis data.
  - (c) Any changes made in laboratory's LIMS system:
    - Must be documented and traceable.
    - If made by staff of an affiliate lab, written permission from the home lab to make the changes (email approval is sufficient) is required.
    - No corrections may be made in another laboratories system without their knowledge.
  - (d) Data qualifiers in laboratory reports must only be corrected, edited, etc. by the staff at the host laboratory.
  - (e) Full analytical data "View" only permissions may be granted to outside Project Management and Sales staff. Search permissions may also be granted so status may be checked.
  - (f) All qualifiers must be approved by QA staff before adding to standard reference tables.
  - (g) Please contact Corporate QA or IT staff if you have any questions regarding implementation or interpretation of this policy.**

**20.13.1.2 Ensure Information Availability:** Protection against loss of information or service through scheduled back-ups, secure storage of media, line filter, Uninterruptible Power Supply (UPS), and maintaining older versions of software as revisions are implemented.

- Insured by timely backup procedures on reliable backup media, stable file server network architecture, and UPS protection
- UPS Protection:
  - Each fileserver is protected by an appropriate power protection/backup unit. In the event of a power outage, there is approximately 15-30 minutes of up-time for the servers prior to shutdown. This allows for proper shutdown procedures to be followed with the file servers.
- File Server Architecture
  - All files are maintained on multiple Windows 2000 or newer servers which are secured physically in the Information Technology office. Access to these servers is limited to members of the Information Technology staff.
  - All supporting software is maintained for at least 5 years from the last raw data generated using that software. [Length of time is dependent on local regulations or client requirements (e.g., OVAP requires 10 years).]

- System Back-up Overview and Procedures
  - Data from both servers and instrument attached PC's are backed up and purged in compliance with the corporate back-up policy.
  - A Maintenance Plan has been defined to create a daily archive of all data within the LIMS database to a backup location. This backup is initiated automatically by either the database or back-up system.
  - Backup tapes will be stored in compliance with the corporate Data Backup Policy. Backup verifications are carried out in accordance with the corporate Data Backup Policy.
  - Instrument data back-ups are verified on a periodic basis by the QA department when performing electronic data audits. The audit takes place on data that has been moved to a back-up location ensuring that it has been moved.

**20.13.1.3 Maintain Confidentiality:** Ensure data confidentiality through physical access controls, and use encryption when electronically transmitting data.

- All servers are located in a secure area of the IT department offices. Access to the servers is limited to IT staff members, the lab director, and the manager of customer service.
- The company website contains SSL (Secure Socket Layer) encryption for secure website sessions and data transfers.
- Electronic documents such as PDF files and electronic data deliverables will be made available to clients via the secure web site. The logon page for this web site contains an agreement that the customer must accept before they will be logged on which states that the customer agrees not to alter any electronic data made available to them.
- If electronic documents are made available outside of the web site, the customer must sign an agreement in advance that states they will not alter the data in any way.

**20.13.2 Data Reduction**

The complexity of the data reduction depends on the analytical method and the number of discrete operations involved (e.g., extractions, dilutions, instrument readings and concentrations). The analyst calculates the final results from the raw data or uses appropriate computer programs to assist in the calculation of final reportable values.

For manual data entry, e.g., Wet Chemistry, the data is reduced by the analyst and then verified by the Department Manager or alternate analyst prior to updating the data in LIMS. The data review checklists are signed by both the analyst and alternate reviewer to confirm the accuracy of the manual entry(s).

Manual integration of peaks will be documented and reviewed and the raw data will be flagged in accordance with the TestAmerica Corporate SOP CA-Q-S-002, *Acceptable Manual Integration Practices* and the TestAmerica West Sacramento Addendum.

Analytical results are reduced to appropriate concentration units specified by the analytical method, taking into account factors such as dilution, sample weight or volume, etc. Blank correction will be applied only when required by the method or per manufacturer's indication; otherwise, it should not be performed. Calculations are independently verified by appropriate laboratory staff.

Calculations and data reduction steps for various methods are summarized in the respective analytical SOPs or program requirements.

**20.13.2.1** All raw data must be retained in the worklist folder, computer file (if appropriate), and/or runlog. All criteria pertinent to the method must be recorded. The documentation is recorded at the time observations or calculations are made and must be signed or initialed/dated (month/day/year). It must be easily identifiable who performed which tasks if multiple people were involved.

**20.13.2.2** In general, concentration results are reported in milligrams per liter (mg/l) or micrograms per liter ( $\mu\text{g/l}$ ) for liquids and milligrams per kilogram (mg/kg) or micrograms per kilogram ( $\mu\text{g/kg}$ ) for solids. The units "mg/l" and "mg/kg" are the same as "parts per million (ppm)". The units " $\mu\text{g/l}$ " and " $\mu\text{g/kg}$ " are the same as "parts per billion (ppb)." For values greater than 10,000 mg/l, results can be reported in percent, i.e., 10,000 mg/l = 1%.

- Several environmental methods, such as color, turbidity, conductivity, use very specific, non-concentration units to report results (e.g., NTU, umhos/cm etc).
- Air methods are reported in units of total ug/sample or total ng/sample.
- Occasionally, the client requests that results be reported in units which take into account the measured flow of water or air during the collection of the sample. When they provide this information, the calculations can be performed and reported.

**20.13.2.3** In reporting, the analyst or the instrument output records the raw data result using values of known certainty plus one uncertain digit. If final calculations are performed external to LIMS, the results should be entered in LIMS with at least three significant figures. In general, results are reported to 2 significant figures on the final report.

**20.13.2.4** For those methods that do not have an instrument printout or an instrumental output compatible with the LIMS System, the raw results and dilution factors are entered directly into LIMS by the analyst, and the software calculates the final result for the analytical report. LIMS has a defined significant figure criterion for each analyte.

**20.13.2.5** The laboratory strives to import data directly from instruments or calculation spreadsheets to ensure that the reported data are free from transcription and calculation errors. For those analyses with an instrumental output compatible with the LIMS, the raw results and dilution factors are transferred into LIMS electronically after reviewing the quantitation report, and removing unrequested or poor spectrally-matched compounds. The analyst prints a copy of what has been entered to check for errors. This printout and the instrument's printout of calibrations, concentrations, retention times, chromatograms, and mass spectra, if applicable, are retained with the data file.

### **20.13.3 Logbook / Worksheet Use Guidelines**

Logbooks and worksheets are filled out 'real time' and have enough information on them to trace the events of the applicable analysis/task. (e.g. calibrations, standards, analyst, sample ID, date, time on short holding time tests, temperatures when applicable, calculations are traceable, etc.)

- Corrections are made following the procedures outlined in Section 13.
- Logbooks are controlled by the QA department. A record is maintained of all logbooks in the lab.
- Unused portions of pages must be “Z”d out, signed and dated.
- Worksheets are created with the approval of the Technical Director/QA Manager at the facility. The QA Manager controls all worksheets following the procedures in Section 6.

#### **20.13.4 Review / Verification Procedures**

Review procedures are out lined in several SOPs and Policies:

- WS-PQA-003, “Quality Control Program”
- QA-012-SAC, “Technical Data Review Requirements”
- SAC-PM-0004, “Final Report Assembly and Third Level Data Review”

These procedures ensure that reported data are free from calculation and transcription errors, that QC parameters have been reviewed and evaluated before data is reported. The laboratory also utilizes the Corporate SOP No. CA-Q-S-002, “Acceptable Manual Integration Practices” and the TestAmerica West Sacramento Addendum to CA-Q-S-002, which discuss Manual Integrations to ensure the authenticity of the data. The general review concepts are discussed below, more specific information can be found in the SOPs.

**20.13.4.1** The data review process at TestAmerica West Sacramento starts at the Sample Control level. Sample Control personnel review chain-of-custody forms and input the sample information and required analyses into a computer LIMS. The Sample Control Supervisor reviews the transaction of the chain-of-custody forms and the inputted information. The Project Managers perform final review of the chain-of-custody forms and inputted information.

**20.13.4.2** The next level of data review occurs with the Analysts. As results are generated, analysts review their work to ensure that the results generated meet QC requirements and relevant EPA methodologies. The Analysts transfer the data into the LIMS and add data qualifiers if applicable (see Appendix 7 for a list of common data qualifiers). To ensure data compliance, a different analyst performs a second level of review. Second level review is accomplished by checking reported results against the raw data and evaluating the results for accuracy. During the second level review, blank runs, QA/QC check results, continuing calibration results, laboratory control samples, sample data, qualifiers and spike information are evaluated. One hundred percent of all sample data from manual methods and from automated methods, all GC/MS spectra and all manual integrations are reviewed. Manual integrations are also electronically reviewed utilizing auditing software to help ensure compliance to ethics and manual integration policies. Issues that deem further review include the following:

- QC data are outside the specified control limits for accuracy and precision
- Reviewed sample data does not match with reported results

- Unusual detection limit changes are observed
- Samples having unusually high results
- Samples exceeding a known regulatory limit
- Raw data indicating some type of contamination or poor technique
- Inconsistent peak integration
- Transcription errors
- Results outside of calibration range

**20.13.4.3** Unacceptable analytical results may require reanalysis of the samples. Any problems are brought to the attention of the Laboratory Director, Project Manager, Quality Assurance Manager, Operations Manager, or Department Manager for further investigation. Corrective action is initiated whenever necessary.

**20.13.4.4** The results are then entered or directly transferred into the computer database and a hard copy (or .pdf) is printed for the client.

**20.13.4.5** As a final review prior to the release of the report, the Project Manager reviews the results for appropriateness and completeness. This review and approval ensures that client requirements have been met and that the final report has been properly completed. The process includes, but is not limited to, verifying that chemical relationships are evaluated, COC is followed, cover letters/ narratives are present, flags are appropriate, and project specific requirements are met. The following are some examples of chemical relationships that are reviewed (if data is available):

- Total Results are  $\geq$  Dissolved results (e.g. metals)
- Total Solids (TS)  $\geq$  TDS or TSS
- TKN  $\geq$  Ammonia
- Total Phosphorus  $\geq$  Orthophosphate
- COD  $\geq$  TOC
- Total cyanide  $\geq$  Amenable Cyanide
- TDS  $\geq$  individual anions

**20.13.4.6** The Project Manager then signs the final report. (*Also see Section 26 on Reporting Results*). When complete, the report is sent out to the client.

**20.13.4.7** A visual summary of the flow of samples and information through the laboratory, as well as data review and validation, is presented in Figure 20-3.

### **20.13.5 Manual Integrations**

Computerized data systems provide the analyst with the ability to re-integrate raw instrument data in order to optimize the interpretation of the data. Though manual integration of data is an invaluable tool for resolving variations in instrument performance and some sample matrix problems, when used improperly, this technique would make unacceptable data appear to meet quality control acceptance limits. Improper re-integrations lead to legally indefensible data, a poor reputation, or possible laboratory decertification. Because guidelines for re-integration of data are not provided in the methods and most methods were written prior to widespread implementation of computerized data systems, the laboratory trains all analytical staff on proper manual integration techniques using SOP CA-Q-S-002 and the laboratory addendum as the guidelines.

- 20.13.5.1** The analyst must adjust baseline or the area of a peak in some situations, for example when two compounds are not adequately resolved or when a peak shoulder needs to be separated from the peak of interest. The analyst must use professional judgment and common sense to determine when manual integrating is required. Analysts are encouraged to ask for assistance from a senior analyst or manager when in doubt.
- 20.13.5.2** Analysts shall not increase or decrease peak areas for the sole purpose of achieving acceptable QC recoveries that would have otherwise been unacceptable. The intentional recording or reporting of incorrect information (or the intentional omission of correct information) is against company principals and policy and is grounds for immediate termination.
- 20.13.5.3** Client samples, performance evaluation samples, and quality control samples are all treated equally when determining whether or not a peak area or baseline should be manually adjusted.
- 20.13.5.4** All manual integrations receive a second level review. Manual integrations must be indicated on an expanded scale “after” chromatograms such that the integration performed can be easily evaluated during data review. Expanded scale “before” chromatograms are also required for all manual integrations on QC parameters (calibrations, calibration verifications, laboratory control samples, internal standards, surrogates, etc.) unless the laboratory has another documented corporate approved procedure in place that can demonstrate an active process for detection and deterrence of improper integration practices.

**Figure 20-1.**  
**Example - Demonstration of Capability Documentation**

## ***Demonstration of Capability Certification Statement***

**TestAmerica West Sacramento**

880 Riverside Parkway  
West Sacramento, CA 95605  
(916) 373-5600      SOP:

**Date:**

Method:

Matrix: Aqueous

Analyst(s):

---

We, the undersigned, CERTIFY that:

- 1: The analyst(s) identified above, using the cited test method, with the specifications in the cited SOP, which is in use at the facility for the analysis of samples under the TestAmerica West Sacramento Quality Assurance Manual, has met the Demonstration of Capability.
  
- 2: The test method was performed by the analyst(s) identified on this certification following the TestAmerica West Sacramento SOP.
  
- 3: A copy of the laboratory-specific SOP is available for all personnel on-site.
  
- 4: The data associated with the demonstration of capability are true, accurate, complete and self-explanatory (\*). These data are attached to this certification statement.
  
- 5: All raw data (including a copy of this certification form) necessary to reconstruct and validate these analyses have been retained at the facility, and that the associated information is well organized and available for review by authorized inspectors.

Comments/ Observations:

---

Karla Buechler  
Technical Director

\_\_\_\_\_  
Technical Director Signature

\_\_\_\_\_  
Date

Pamela Schemmer  
QA Manager

\_\_\_\_\_  
QA Manager Signature

\_\_\_\_\_  
Date

**Figure 20-2.**

**Example - New Instrument / Method / Additional Analyte Checklist**

**TESTAMERICA WEST SACRAMENTO  
INSTRUMENT/METHOD VALIDATION CHECKLIST**

Instrument Type: \_\_\_\_\_ Model#: \_\_\_\_\_ Serial #: \_\_\_\_\_

Lab Equip Code: \_\_\_\_\_ LIMS Equip Code: \_\_\_\_\_

Method(s) \_\_\_\_\_ Analytes (attach list) \_\_\_\_\_

Matrices:  Water  Soil  Tissue  Air (specify) \_\_\_\_\_  Other \_\_\_\_\_

Instrument Installation Date: \_\_\_\_\_

Installed By: \_\_\_\_\_

Instrument installed per specifications. Operational and functional per install guidelines.

Signature/Date of installer: \_\_\_\_\_

\_\_\_\_\_ Standard Operating Procedure ID \_\_\_\_\_

\_\_\_\_\_ Evaluation of Selectivity. As applicable: e.g. Retention Time Window Study, second column confirmation, Interelement correction checks, spectral or fluorescence profiles, etc

\_\_\_\_\_ Initial Calibration Curve (Include second source and Tune verification or similar (e.g. degradation checks) if applicable)

\_\_\_\_\_ Demonstration of Capability (DOC)

Appropriate MDL's/ MDL checks as applicable per method complete: \_\_\_\_\_

\*MDL's must be forwarded to the QA Dept. for Validation to be considered complete.

\_\_\_\_\_ Acceptable PT sample(s) if available

Outstanding items yet to be completed (If applicable): \_\_\_\_\_

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

Completion Date: \_\_\_\_\_

Signature/Date Lab Representative: \_\_\_\_\_



Instrument passes all initial required lab checks and calibrations as appropriate for method of analysis: \_\_\_\_\_

In-Service Date: \_\_\_\_\_

Signature/Date of Lab Representative: \_\_\_\_\_

Signature/Date of QA Representative: \_\_\_\_\_

Figure 20-3.

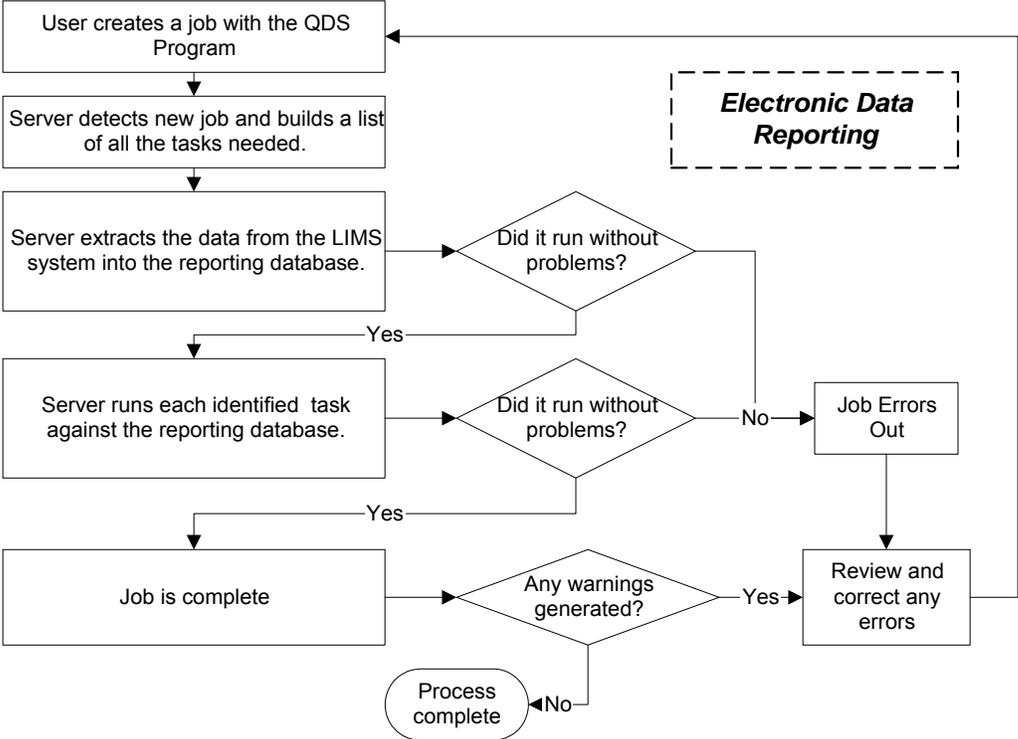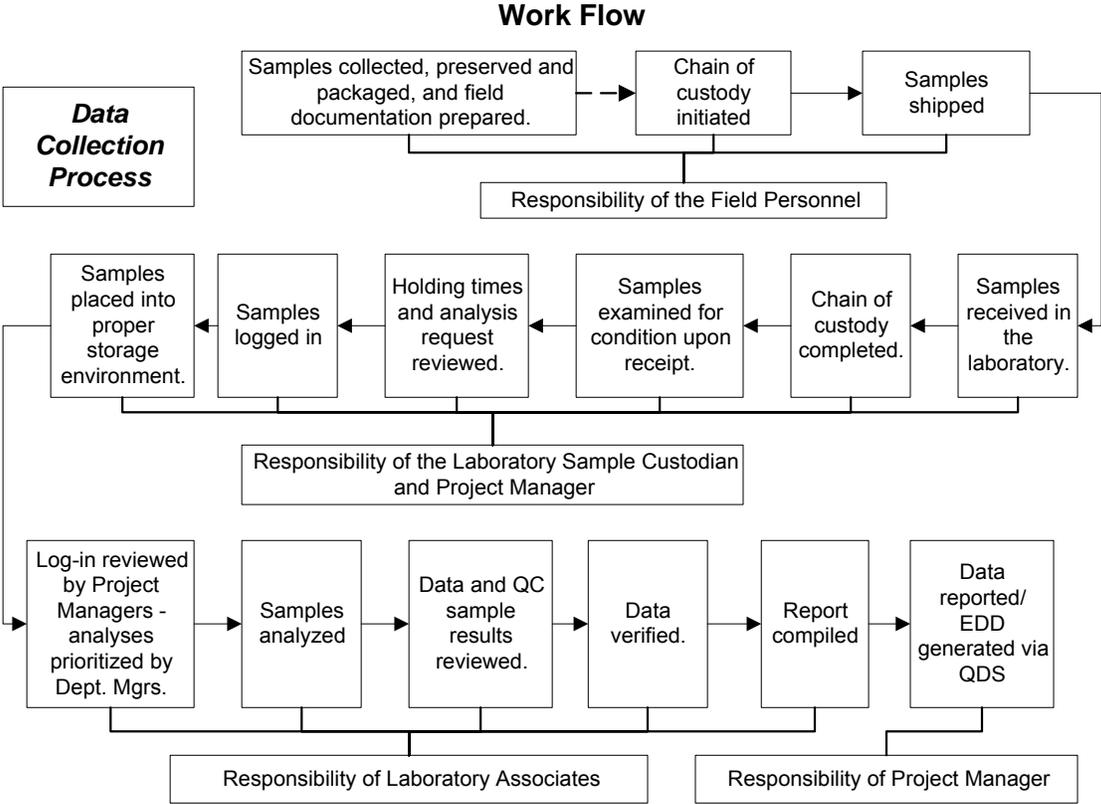

**SECTION 21**  
**EQUIPMENT (AND CALIBRATIONS)**  
**(NELAC 5.5.5)**

**21.1**      **OVERVIEW**

TestAmerica purchases the most technically advanced analytical instrumentation for sample analyses. Instrumentation is purchased on the basis of accuracy, dependability, efficiency and sensitivity. Each laboratory is furnished with all items of sampling, preparation, analytical testing and measurement equipment necessary to correctly perform the tests for which the laboratory has capabilities. Each piece of equipment is capable of achieving the required accuracy and complies with specifications relevant to the method being performed. Before being placed into use, the equipment (including sampling equipment) is calibrated and checked to establish that it meets its intended specification. The calibration routines for analytical instruments establish the range of quantitation. Calibration procedures are specified in laboratory SOPs. A list of laboratory equipment and instrumentation is presented in Table 21-1.

Equipment is only operated by authorized and trained personnel. Manufacturers' instructions for equipment use are readily accessible to all appropriate laboratory personnel.

**21.2**      **PREVENTIVE MAINTENANCE**

**21.2.1**      TestAmerica West Sacramento follows a well-defined program to ensure proper equipment operation and to prevent the failure of laboratory equipment or instrumentation during use. This program of preventive maintenance helps to avoid delays due to instrument failure.

**21.2.2**      Routine preventive maintenance procedures and frequency, such as lubrication, cleaning, and replacements, should be performed according to the procedures outlined in the manufacturer's manual. Qualified personnel must also perform maintenance when there is evidence of degradation of peak resolution, a shift in the calibration curve, loss of sensitivity, or failure to continually meet one of the quality control criteria.

**21.2.2.1**      Calibrations, routine maintenance, and adjustments are part of the analysts' and Department Managers' responsibilities. However, service contracts may be in place for some instruments to cover any major repairs.

**21.2.2.2**      High purity gases, reagents, and spare parts are kept on hand to minimize repair time and optimize instrument performance.

**21.2.3**      Table 21-2 summarizes the schedule for routine maintenance. It is the responsibility of each Department Manager to ensure that instrument maintenance logs are kept for all equipment in his/her department. Preventative maintenance procedures may also be outlined in analytical SOPs or instrument manuals. (Note: for some equipment, the log used to monitor performance is also the maintenance log. Multiple pieces of equipment may share the same log as long as it is clear as to which instrument is associated with an entry.)

**21.2.4**      Instrument maintenance logs are controlled and are used to document instrument problems, instrument repair and maintenance activities. Maintenance logs shall be kept for all

major pieces of equipment. Instrument maintenance logs may also be used to specify instrument parameters.

**21.2.4.1** Documentation must include all major maintenance activities such as contracted preventive maintenance and service and in-house activities such as the replacement of electrical components, lamps, tubing, valves, columns, detectors, cleaning and adjustments.

**21.2.4.2** Each entry in the instrument log includes the Analyst's initials, the date, a detailed description of the problem (or maintenance needed/scheduled), a detailed explanation of the solution or maintenance performed, and a verification that the equipment is functioning properly (state what was used to determine a return to control. e.g. CCV run on 'date' was acceptable, or instrument recalibrated on 'date' with acceptable verification, etc.).

**21.2.4.3** When maintenance or repair is performed by an outside agency, service receipts detailing the service performed can be affixed into the logbooks adjacent to pages describing the maintenance performed. This stapled in page must be signed across the page entered and the logbook so that it is clear that a page is missing if only half a signature is found in the logbook.

**21.2.5** In addition, the maintenance records contain:

- The identification of the instrument/equipment (instrument's Serial Number and Model Number)
- The date the instrument/equipment was put into use.
- If available, the condition when the instrument was received (e.g. new, used, reconditioned).
- Any maintenance procedures and frequency or a reference to their location in the QAM.

**21.2.6** If an instrument requires repair (subjected to overloading or mishandling, gives suspect results, or otherwise has shown to be defective or outside of specified limits) it shall be taken out of operation and tagged as out of service or otherwise isolated until such a time as the repairs have been made and the instrument can be demonstrated as operational by calibration and/or verification or other test to demonstrate acceptable performance. The laboratory shall examine the effect of this defect on previous analyses (refer to Sections 12 and 13).

**21.2.7** In the event of equipment malfunction that cannot be resolved, service shall be obtained from the instrument vendor manufacturer, or qualified service technician, if such a service can be tendered. If on-site service is unavailable, arrangements shall be made to have the instrument shipped back to the manufacturer for repair. Back up instruments, which have been approved, for the analysis shall perform the analysis normally carried out by the malfunctioning instrument. If the back up is not available and the analysis cannot be carried out within the needed timeframe, the samples shall be subcontracted using the procedures outlined in Section 8.

If an instrument is sent out for service or transferred to another facility, it must be recalibrated and verified (including new initial MDL study) prior to return to lab operations.

### **21.3 SUPPORT EQUIPMENT**

This section applies to all devices that may not be the actual test instrument, but are necessary to support laboratory operations. These include but are not limited to: balances, ovens, refrigerators, freezers, incubators, water baths, field sampling devices, temperature measuring devices, thermal/pressure sample preparation devices and volumetric dispensing devices if quantitative results are dependent on their accuracy, as in standard preparation and dispensing or dilution into a specified volume. All raw data records associated with the support equipment are retained to document instrument performance.

#### **21.3.1 Weights and Balances**

The accuracy of the balances used in the laboratory is checked every working day, before use. All balances are placed on stable counter tops.

Each balance is checked prior to use with at least two certified ASTM type 1 weights spanning its range of use (weights that have been calibrated to ASTM type 1 weights may also be used for daily verification). ASTM type 1 weights used only for calibration of other weights (and no other purpose) are inspected for corrosion, damage or nicks at least annually and if no damage is observed, they are calibrated at least every 5 years by an outside calibration laboratory. Any weights (including ASTM Type 1) used for daily balance checks or other purposes are recalibrated/recertified annually to NIST standards (this may be done internally if laboratory maintains "calibration only" ASTM type 1 weights).

All balances are serviced annually by a qualified service representative, who supplies the laboratory with a certificate that identifies traceability of the calibration to the NIST standards.

All of this information is recorded in logs, and the recalibration/recertification certificates are kept on file. See SOP No. SAC-QA-0041, "Calibration and Calibration Check of Balances" for more details.

#### **21.3.2 pH, Conductivity, and Turbidity Meters**

The pH meters used in the laboratory are accurate to  $\pm 0.1$  pH units, and have a scale readability of at least 0.05 pH units. The meters automatically compensate for the temperature, and are calibrated with at least two working range buffer solutions before each use.

Conductivity meters are also calibrated before each use with a known standard to demonstrate the meters do not exceed an error of 1% or one umhos/cm.

Turbidity meters are also calibrated before each use. All of this information is documented in logs.

Consult pH and Conductivity, and Turbidity SOPs for further information.

#### **21.3.3 Thermometers**

All thermometers are calibrated on an annual basis with a NIST-traceable thermometer. IR thermometers, digital probes, and thermocouples are calibrated quarterly.

The NIST thermometer is recalibrated every five years (unless the thermometer has been exposed to temperature extremes or apparent separation of internal liquid) by an approved outside service and the provided certificate of traceability is kept on file. The NIST thermometer has increments of 0.2 °C, and has a range applicable to all method and certification requirements. The NIST traceable thermometer is used for no other purpose than to calibrate other thermometers.

All of this information is documented in logbooks. Monitoring method-specific temperatures, including incubators, heating blocks, water baths, and ovens, is documented in method-specific logbooks. More information on this subject can be found in SOP No. SAC-QA-0016, "Thermometer Calibration."

#### **21.3.4 Refrigerators/Freezer Units, Waterbaths, Ovens and Incubators**

The temperatures of all refrigerator units and freezers used for sample storage are monitored 7 days a week; and each working day for units used for standard storage.

Ovens, waterbaths and incubators are monitored on days of use.

All of this equipment has a unique identification number, and is assigned a unique thermometer for monitoring.

Sample storage refrigerator temperatures are kept between  $> 0^{\circ}\text{C}$  and  $\leq 6^{\circ}\text{C}$ .

Specific temperature settings/ranges for other refrigerators, ovens waterbaths, and incubators can be found in method specific SOPs.

All of this information is documented on Daily Temperature Sheets.

#### **21.3.5 Autopipettors, Dilutors, and Syringes**

Mechanical volumetric dispensing devices including burettes (except Class A Glassware) are checked for accuracy at least quarterly. Glass micro-syringes are considered the same as Class A glassware.

The laboratory maintains a sufficient inventory of autopipettors, and dilutors of differing capacities that fulfill all method requirements.

These devices are given unique identification numbers, and the delivery volumes are verified gravimetrically, at a minimum, on a quarterly basis.

For those dispensers that are not used for analytical measurements, a label is applied to the device stating that it is not calibrated. Any device not regularly verified can not be used for any quantitative measurements. See SOP SAC-QA-0004, "Maintenance and Calibration Check of Fixed and Adjustable Volume Autopipettors, Autodispensers and Volumetric Containers".

Micro-syringes are purchased from Hamilton Company. Each syringe is traceable to NIST. The laboratory keeps on file an "Accuracy and Precision Statement of Conformance" from Hamilton attesting established accuracy.

### **21.3.6 Autoclaves**

Autoclaves used for sample digestion are capable of maintaining conditions of 15 psi at 120°C for 15 minutes. The temperature of the autoclave is verified quarterly.

## **21.4 INSTRUMENT CALIBRATIONS**

Calibration of analytical instrumentation is essential to the production of quality data. Strict calibration procedures are followed for each method. These procedures are designed to determine and document the method detection limits, the working range of the analytical instrumentation and any fluctuations that may occur from day to day.

Sufficient raw data records are retained to allow an outside party to reconstruct all facets of the initial calibration. Records contain, but are not limited to, the following: calibration date, method, instrument, analyst(s) initials or signatures, analysis date, analytes, concentration, response, type of calibration (Avg RF, curve, or other calculations that may be used to reduce instrument responses to concentration.)

Sample results must be quantitated from the initial calibration and may not be quantitated from any continuing instrument calibration verification unless otherwise required by regulation, method or program. If the initial calibration results are outside of the acceptance criteria, corrective action is performed and any affected samples are reanalyzed if possible. If the reanalysis is not possible, any data associated with an unacceptable initial calibration will be reported with appropriate data qualifiers (refer to Section 13).

**Note:** Instruments are calibrated initially and as needed after that and at least annually; however, the annual requirement does not apply to Isotope dilution methods.

### **21.4.1 CALIBRATION STANDARDS**

Calibration standards are prepared using the procedures indicated in the Reagents and Standards section of the determinative method SOP. However, the general procedures are described below.

**21.4.1.1** For each analyte and surrogate (if applicable) of interest, prepare calibration standards at the minimum number of concentrations as stated in the analytical methods. If a reference or mandated method does not specify the number of calibration standards, the minimum number is three, not including blanks or a zero standard. All of the standard solutions are prepared using Class A volumetric glassware, calibrated pipettes, and/or microsyringes and appropriate laboratory quality solvents and stock standards.

**21.4.1.2** Standards for instrument calibration are obtained from a variety of sources. All standards are traceable to NIST whenever possible. Dilution standards are prepared from stock standards purchased from commercial suppliers. A standard log or program is maintained for each department, containing concentration, date of receipt, date of standard preparation, any dilutions made, lot number, supplier, type of solvent and a unique code number to identify the standard.

- 21.4.1.3** The lowest concentration calibration standard that is analyzed during an initial calibration must be at or below the stated reporting limit for the method based on the final volume of extract (or sample).
- 21.4.1.4** The other concentrations define the working range of the instrument/method or correspond to the expected range of concentrations found in actual samples that are also within the working range of the instrument/method. Results of samples not bracketed by initial instrument calibration standards (within calibration range to 3 significant figures) must be reported as having less certainty, e.g., defined qualifiers or flags (additional information may be included in the case narrative). The lowest calibration standard must be at or below the reporting limit. The exception to these rules is ICP methods or other methods where the referenced method does not specify two or more standards.
- 21.4.1.5** Given the number of target compounds addressed by some of the organic methods, it may be necessary to prepare several sets of calibration standards, each set consisting of the appropriate number of solutions at different concentrations. The initial calibration will then involve the analysis of each of these sets of the appropriate number of standards.
- 21.4.1.6** All initial calibrations are verified with a standard obtained from a second source and traceable to a national standard, when available (or vendor certified different lot if a second source is not available). For unique situations, such as air analysis where no other source or lot is available, a standard made by a different analyst would be considered a second source. This verification occurs immediately after the calibration curve has been analyzed, and before the analysis of any samples.

**21.4.2** **CALIBRATION FOR ORGANIC METHODS (GC, HPLC, GC/MS)**

- 21.4.2.1** Many of the organic analytical methods utilize an internal standard calibration (GCMS and some GC). Because of the complex nature of the multippeak chromatograms produced by the method, some instruments necessitate the use of external standard calibration (most GC and HPLC). Surrogate compounds are included in the calibration processes for all appropriate organic analyses. For more details on the calibration types listed below, refer to SOP No. CA-Q-S-005, Calibration Curves.
- 21.4.2.2** Once the operating parameters have been established according to the method, each instrument is calibrated for the appropriate method. The analyst prepares five or more standard solutions at various concentrations containing all of the analytes of interest, internal standards, and surrogates that are appropriate for the method. Note: There are a several EPA methods that have different requirements and are exceptions (e.g. EPA 547) where a minimum of 3 calibration standards are prepared and analyzed.
- 21.4.2.3** The standard solutions are introduced into the instrument in the same manner as samples are; whether it be by direct injection, by headspace analysis, or by purge and trap. The calibration factor (CF) for methods that use external standards, and

the response factor (RF) for methods that use internal standards are calculated for the five standards.

- External standard calibration involves comparison of instrument responses from the sample to the responses from the target compounds in the calibration standards. Sample peak areas (or peak heights) are compared to peak areas (or heights) of the standards. The ratio of the response to the amount of analyte in the calibration standard is defined as the Calibration factor (CF).
- Internal standard calibration involves the comparison of instrument responses from the target compounds in the sample to the responses of specific standards added to the sample or sample extract prior to injection. The ratio of the peak area (or height) of the target compound in the sample or sample extract to the peak area (or height) of the internal standard in the sample or sample extract is compared to a similar ratio derived for each calibration standard. The ratio is termed the response factor (RF), and may also be known as a relative response factor in other methods.

In many cases, internal standards are recommended. These recommended internal standards are often brominated, fluorinated, or stable isotopically labeled analogs of specific target compounds, or are closely related compounds whose presence in environmental samples is highly unlikely. The use of specific internal standards is available in the method SOP.

Whichever internal standards are employed, the analyst needs to demonstrate that the measurement of the internal standard is not affected by method analytes and surrogates or by matrix interferences. In general, internal standard calibration is not as useful for GC and HPLC methods with non-MS detectors because of the inability to chromatographically resolve many internal standards from the target compounds. The use of MS detectors makes internal standard calibration practical because the masses of the internal standards can be resolved from those of the target compounds even when chromatographic resolution cannot be achieved.

When preparing calibration standards for use with internal standard calibration, add the same amount of the internal standard solution to each calibration standard, such that the concentration of each internal standard is constant across all of the calibration standards, whereas the concentrations of the target analytes will vary. The internal standard solution will contain one or more internal standards and the concentration of the individual internal standards may differ within the spiking solution (e.g., not all internal standards need to be at the same concentration in this solution). The mass of each internal standard added to each sample extract immediately prior to injection into the instrument or to each sample prior to purging must be the same as the mass of the internal standard in each calibration standard. The volume of the solution spiked into sample extracts should be such that minimal dilution of the extract occurs (e.g., 10  $\mu$ L of solution added to a 1 mL final extract results in only a negligible 1% change in the final extract volume which can be ignored in the calculations).

An ideal internal standard concentration would yield a response factor of 1 for each analyte. However, this is not practical when dealing with more than a few target analytes. Therefore, as a general rule, the amount of internal standard should produce an instrument response (e.g., area counts) that is no more than 100 times that produced by the lowest concentration of the least responsive target analyte associated with the internal standard. This should result in a

minimum response factor of approximately 0.01 for the least responsive target compound. Refer to SOP No. CA-Q-S-005, Calibration Curves, for specific calculations.

**21.4.2.4** Policies regarding the use of calibration standard results for creating the calibration curve are as follows:

- A low calibration standard may be excluded from the calibration if the signal-to-noise ratio or spectral criteria are not suitable. The reporting level must be elevated to be the lowest calibration standard used for calibration.
- The upper calibration standard may be excluded if it saturates the detector or is obviously becoming non-linear. Any sample exceeding the upper standard used in the calibration must be diluted and re-analyzed.
- Mid-calibration standards may not be excluded unless an obvious reason is found, i.e., cracked vial, incorrectly made, etc. The failed standard should be re-run immediately and inserted into the initial calibration. If not useful, recalibration is required.

#### **21.4.2.5 Percent RSD Corrective Action**

Given the potentially large numbers of analytes that may be analyzed in some methods, it is likely that some analytes may exceed the acceptance limit for the RSD for a given calibration. In those instances, the following steps are recommended, but not required.

**21.4.2.5.1** The first step is generally to check the instrument operating conditions. This option will apply in those instances where a linear instrument response is expected. It may involve some trade-offs to optimize performance across all target analytes. For instance, changes to the operating conditions necessary to achieve linearity for problem compounds may cause the RSD for other compounds to increase, but as long as all analytes meet the RSD limits for linearity, the calibration is acceptable.

**21.4.2.5.2** If the RSD for any analyte is greater than the applicable acceptance criteria in the applicable analytical method or method SOP, the analyst may wish to review the results (area counts, calibration or response factors, and RSD) for those analytes to ensure that the problem is not associated with just one of the initial calibration standards. If the problem appears to be associated with a single standard, that one standard may be reanalyzed and the RSD recalculated. Replacing the standard may be necessary in some cases.

**21.4.2.5.3** A third alternative is to narrow the calibration range by replacing one or more of the calibration standards with standards that cover a narrower range. If linearity can be achieved using a narrower calibration range, document the calibration linearity, and proceed with analyses. The changes to the upper end of the calibration range will affect the need to dilute samples above the range, while changes to the lower end will affect the overall sensitivity of the method. Consider the regulatory limits or action levels associated with the target analytes when adjusting the lower end of the range.

**Note:** When the purpose of the analysis is to demonstrate compliance with a specific regulatory limit or action level, the laboratory must ensure that the method quantitation limit is at least as low as the regulatory limit or action level.

**21.4.2.6** Alternatively, the least squares regression may be used to determine linearity. A five point line must result in a correlation coefficient ( $r$ ) of 0.990 or better using the least squares method to be considered acceptable. In many cases it may be preferred that the curves be forced through zero (not to be confused with including the origin as an additional data point, which is not allowed). **Note:** EPA method 8000B does not allow forcing through zero however the agency has reevaluated this position and has since changed this stance to allow forcing through zero. In addition, from EPA Method 8000C: "However, the use of a linear regression or forcing the regression through zero may NOT be used as a rationale for reporting results below the calibration range demonstrated by the analysis of the standards.").

**21.4.2.7** Instead of a linear curve model (either Average RF or least squares regression), a second order curve (Quadratic) may be used (and preferred) as long as it contains at least six data points. As a rule of thumb, if there is a consistent trend in RFs (or CFs) in the calibration curve, either up or down, then quadratic curve fit may be indicated as the preferred calibration routine for that analyte. The coefficient of determination (COD or  $r^2$ ) for the quadratic curve must be at least 0.99 for it to be considered acceptable. For more details on the calculations see Calibration Curve SOP CA-Q-S-005. Some limitations on the use of Quadratic Curve fits:

**21.4.2.7.1** Care **MUST** be exercised to assure that the results from this equation are real, positive, and fit the range of the initial calibration.

**21.4.2.7.2** They **may not** be used to mask instrument problems that can be corrected by maintenance. (Not to be used where the analyte is normally found to be linear in a properly maintained instrument).

**21.4.2.7.3** They **may not** be used to compensate for detector saturation. If it is suspected that the detector is being saturated at the high end of the curve, remove the higher concentration standards from the curve and try a 1<sup>st</sup> order fit or average RF.

### **21.4.3 Calibration for Inorganic Analyses**

EPA Method 7000 from EPA SW-846 is a general introduction to the quality control requirements for metals analysis. For inorganic methods, quality control measures set out in the individual methods and in the *Standard Methods for the Examination of Water and Wastewater* (20th Edition) may also be included. Standard Operating Procedures for the analysis and the quality control documentation measures are available in the laboratory SOP, which is available on the Intranet.

In general, inorganic instrumentation is calibrated with external standards. Some exceptions would be Inductively Coupled Plasma (ICP), and Inductively Coupled Plasma Mass

Spectrometry (ICPMS). These analyses may use an internal standard to compensate for viscosity or other matrix effects. While the calibration procedures are much the same for inorganics as they are for organics, CFs or RFs are not used. The calibration model in 21.4.2.6 is generally used for most methods, however in some instances the model from section 21.4.2.7 may be used. A correlation coefficient ( $r$ ) of 0.995 or greater must be used to accept a calibration curve generated for an inorganic procedure. Correlation coefficients are determined by computer programs and documented as part of the calibration raw data. Coefficients of calibration curves used for quantitation must be documented as part of the raw data.

**21.4.3.1** "Calibrations" for titrimetric analyses are performed by standardizing the titrants against a primary standard solution. See specific methods in *Standard Methods for the Examination of Water and Wastewater* (20th Edition) for more information.

**21.4.3.2** Spreadsheets that are used for general chemistry calculations must have all cells containing calculations locked to prevent accidental changes to the calculations.

**21.4.3.3** Instrument technologies (e.g. ICP) with validated techniques from the instrument manufacturer or other methods using a zero point and single point calibration require the following:

**21.4.3.3.1** The instrument is calibrated using a zero point and a single point calibration standard.

**21.4.3.3.2** The linear range is established by analyzing a series of standards, one at the reporting limit (RL).

**21.4.3.3.3** Sample results within the established linear range do not need to be qualified.

**21.4.3.3.4** The zero point and single standard is run daily with each analytical batch.

**21.4.3.3.5** A standard at the RL is analyzed daily with each analytical batch and must meet established acceptance criteria.

**21.4.3.3.6** The linearity is verified at a frequency established by the manufacturer or method.

#### **21.4.4**     **Calibration Verification**

The calibration relationship established during the initial calibration must be verified at periodic intervals as specified in the laboratory method SOPs in accordance with the referenced analytical methods and NELAC (2003) standard, Section 5.5.5.10. The process of calibration verification applies to both external standard and internal standard calibration techniques, as well as to linear and non-linear calibration models.

**Note:** The process of calibration verification referred to is fundamentally different from the approach called "calibration" in some methods. As described in those methods, the calibration factors or response factors calculated during calibration are used to update the calibration factors or response factors used for sample quantitation. This approach, while employed in other EPA programs, amounts to a daily single-point calibration, and is neither appropriate nor permitted in SW-846 chromatographic procedures for trace environmental analyses.

**21.4.4.1** Generally, the initial calibrations must be verified at the beginning of each 12-hour analytical shift during which samples are analyzed. (Some methods may specify

more or less frequent verifications). The 12-hour analytical shift begins with the injection of the calibration verification standard (or the MS tuning standard in MS methods). The shift ends after the completion of the analysis of the last sample or standard that can be injected within 12 hours of the beginning of the shift.

**21.4.4.2** A continuing instrument calibration verification (CCV) must be repeated at the beginning and, for methods that have quantitation by external calibration models, at the end of each analytical batch. Some methods have more frequent CCV requirements see specific SOPs. Most Inorganic methods require the CCV to be analyzed after every 10 samples.

**21.4.4.3** The acceptance limits for calibration verifications can be found in each method SOP. As a rule of thumb: GCMS  $\pm 20\%$ , GC and HPLC  $\pm 15\%$ , Inorganics:  $\pm 10$  or  $15\%$ . Actual methods may have wider or tighter limits; see the method SOP for specifics.

**21.4.4.4** If the response (or calculated concentration) for an analyte is within the acceptance limits of the response obtained during the initial calibration, then the initial calibration is considered still valid, and the analyst may continue to use the CF, RF or % drift values from the initial calibration to quantitate sample results.

**21.4.4.5** If the response (or calculated concentration) for any analyte varies from the mean response obtained during the initial calibration by more than the acceptance criteria, then the initial calibration relationship may no longer be valid. If routine corrective action procedures fail to produce a second consecutive (immediate) calibration verification within acceptance criteria, then either the laboratory has to demonstrate performance after corrective action with two consecutive successful calibration verifications, or a new initial instrument calibration must be performed. However, sample data associated with an unacceptable calibration verification may be reported as qualified data under the following special conditions:

**21.4.4.5.1** When the acceptance criteria for the calibration verification are exceeded high, i.e., high bias, and there are associated samples that are non-detects, then those non-detects may be reported. Otherwise, the samples affected by the unacceptable calibration verification shall be reanalyzed after a new calibration curve has been established, evaluated and accepted.

**21.4.4.5.2** When the acceptance criteria for the calibration verification are exceeded low, i.e., low bias, those sample results may be reported if they exceed a maximum regulatory limit/decision level. Otherwise, the samples affected by the unacceptable verification shall be reanalyzed after a new calibration curve has been established, evaluated and accepted. Alternatively, a reporting limit standard may be analyzed to demonstrate that the laboratory can still support non-detects at the reporting limit.

#### **21.4.4.6 Verification of Linear Calibrations**

Calibration verification for linear calibrations involves the calculation of the percent drift or the percent difference of the instrument response between the initial calibration and each subsequent analysis of the verification standard. Use the equations below to calculate % Drift

or % Difference, depending on the procedure specified in the method SOP. Verification standards are evaluated based on the % Difference from the average CF or RF of the initial calibration or based on % Drift or % Recovery if a linear or quadratic curve is used.

The Percent Difference is calculated as follows:

$$\% \text{ Difference} = \frac{(\text{CF}(v) \text{ or } \text{RF}(v)) - (\text{Avg. CF or RF})}{(\text{Avg. CF or RF})} \times 100$$

Where: CF(v) or RF(v) = CF or RF from verification standard  
Avg. CF or RF = Average CF or RF from Initial Calibration.

The Percent Drift is calculated as follows:

$$\% \text{ Drift} = \frac{\text{Result} - \text{True Value}}{\text{True Value}} \times 100$$

The Percent Recovery is calculated as follows:

$$\% \text{ Recovery} = \frac{\text{Result}}{\text{True Value}} \times 100$$

#### **21.4.4.7 Verification of a Non-Linear Calibration**

Calibration verification of a non-linear calibration is performed using the percent drift or percent recovery calculations described in 21.4.4.6 above.

Regardless of whether a linear or non-linear calibration model is used, if initial verification criterion is not met, then no sample analyses may take place until the calibration has been verified or a new initial calibration is performed that meets the specifications listed in the method SOPs. If the calibration cannot be verified after the analysis of a single verification standard, then adjust the instrument operating conditions and/or perform instrument maintenance, and analyze another aliquot of the verification standard. If the calibration cannot be verified with the second standard, then a new initial calibration is performed.

All target analytes and surrogates, including those reported as non-detects, must be included in periodic calibration verifications for purposes of retention time confirmation and to demonstrate that calibration verification criteria are being met.

All samples must be bracketed by periodic analyses of standards that meet the QC acceptance criteria (e.g., calibration and retention time). The frequency is found in the methods SOPs.

**Note:** If an internal standard calibration is being used (basically GCMS) then bracketing standards are not required, only daily verifications are needed unless specified by the method. The results from these verification standards must meet the calibration verification criteria and the retention time criteria (if applicable).

## **21.5 POLICY ON TENTATIVELY IDENTIFIED COMPOUNDS (TICS) – GC/MS ANALYSIS**

For samples containing components not associated with the calibration standards, a library search may be made for the purpose of tentative identification. The necessity to perform this type of identification will be determined by the purpose of the analyses being conducted. Data system library search routines should not use normalization routines that would misrepresent the library or unknown spectra when compared to each other.

**Note:** If the TIC compound is not part of the client target analyte list but is calibrated by the laboratory and is both qualitatively and/or quantitatively identifiable, it will not be reported as a TIC. If the compound is reported on the same form as true TICs, it must be qualified and/or narrated that the reported compound is qualitatively and quantitatively (if verification in control) reported compared to a known standard that is in control (where applicable).

For example, the RCRA permit or waste delisting requirements may require the reporting of non-target analytes. Only after visual comparison of sample spectra with the nearest library searches may the analyst assign a tentative identification. See the GCMS Method SOPs for guidelines for making tentative identifications.

## **21.6 POLICY ON GC/MS TUNING**

Prior to any GCMS analytical sequence, including calibration, the instrument parameters for the tune and subsequent sample analyses within that sequence must be set.

Prior to tuning/auto-tuning the mass spec, the parameters may be adjusted within the specifications set by the manufacturer or the analytical method. These generally don't need any adjustment but it may be required based on the current instrument performance. If the tune verification does not pass it may be necessary to clean the source or perform additional maintenance. Any maintenance is documented in the maintenance log.

**21.6.1** The concentration of the BFB or DFTPP must be at or below the concentrations that are referenced in the analytical methods. Part of the purpose of the tune is to demonstrate sensitivity and analyzing solutions at higher concentrations does not support this purpose. Tune failures may be due to saturation and a lower BFB/DFTPP concentration may be warranted.

**21.6.2** Tune evaluations usually utilize the "Autofind" function and are set up to look at the apex +/- 1 scan and average the three scans. Background correction is required prior to the start of the peak but no more than 20 scans before. Background correction cannot include any part of the target peak.

### **21.6.3 Other Options or if Auto Tune Fails:**

**21.6.3.1** Sometimes the instrument does not correctly identify the apex on some peaks when the peak is not perfectly shaped. In this case, manually identify and average the apex peak +/- 1 scan and background correct as in 21.6.4 above. This is consistent with EPA Methods 8260 and 8270.

- 21.6.3.2** Or the scan across the peak at one half peak height may be averaged and background corrected. This is consistent with Standard Methods 6200, EPA 624 and EPA 625.
- 21.6.3.3** Adjustments such as adjustments to the repeller and ion focus lenses, adjusting the EM Voltage, etc. may be made prior to tune verification as long as all of the subsequent injections in the 12 hour tune cycle are analyzed under the same MS tune settings and it is documented in the run sequence log and/or maintenance log that an adjustment was made. Excessive adjusting (more than 2 tries) without clear documentation is not allowed. Necessary maintenance is performed and documented in the instrument log.
- 21.6.3.4** A single scan at the Apex (only) may also be used for the evaluation of the tune. For SW 846 and EPA 600 series methods, background correction is still required.
- 21.6.3.5** Cleaning the source or other maintenance may be performed and then follow steps for tune evaluation above. Note: If significant maintenance was performed, see methods 8000B or 8000C then the instrument may require recalibration prior to proceeding.
- 21.6.4** Tune evaluation printouts must include the chromatogram and spectra as well as the Tune evaluation information. In addition, the verifications must be sent directly to the printer or pdf file (no screen prints for DFTPP or BFB tunes). This ability should be built into the instrument software.
- 21.6.5** All MS tune settings must remain constant between running the tune check and all other samples. It is recommended that a separate tune method not be used, however a separate method may be used as long as the MS conditions between the methods are the same as the sample analysis method and tracked so any changes that are made to the analysis method are also made to the tune method.

**Table 21-1.**

**Example - Laboratory Equipment and Instrumentation**

Instrument Type	Manufacturer	Model Number	Serial Number	Year Put Into Service	Condition When Received
GC	Agilent	6890N	CN10543080	2005	New
	Hewlett-Packard	6890	US00001087	1997	New
	Hewlett-Packard	6890	US00006442	1997	New
	Hewlett-Packard	6890	US00006441	1997	New
	Hewlett-Packard	6890	US00006438	1997	New
	Agilent	6890N	CN10521082	2005	New
	Hewlett-Packard	6890	US00000311	1997	Used
	Hewlett-Packard	6890	US00006455	1997	New
	Agilent	6890N	CN10521015	2005	New
HPLC	Varian	ProstarV 9065-01384	000498	1998	New
	Waters	2695	B02SM4 915M B02487 788M C02475 452N	2002	New
	Agilent	1100	DE43631861 DE43607107 DE33229050	2005	New
	Agilent	1100	DE43633762 DE43603468 DE43630549	2005	New
	Agilent	1200	DE62961719 JP62360107 DE64762303 DE63055783 DE63064176	2007	New

Instrument Type	Manufacturer	Model Number	Serial Number	Year Put Into Service	Condition When Received
LCMS	Micromass	Quattro	9319	2000	New
	Micromass	Quattro Premier XE	VAB 452	2006	New
	Agilent	6410A Triple Quad	US64810220	2006	New
HIRES	Fisons	VG70	7054	1988	New
	Fisons	VG70	7083	1989	New
	Fisons	Ultima	S176U	1992	New
	Micromass	Ultima	M421	1998	New
	VG Analytical	VG70	US82321724	2001	New
	Micromass	Ultima	M637	2004	New
METALS	Leeman	PS200 II	HG-8008	1998	New
	Leeman	PS200 II	HA-3027	2004	New
	Perkin-Elmer	Optima 4300DV	077N3022401	2003	New
	Perkin-Elmer	ELAN 6000	51950460	1994	New
	Perkin-Elmer	ELAN 6000	4719801	1998	New
	Perkin-Elmer	ELAN 9000 DRC-e	W0170304	2005	Used
GCMS Semivolatiles	Hewlett-Packard	HP 5973	US80221476	1998	New
	Hewlett-Packard	HP 5973	US80321345	1998	New
	Hewlett-Packard	HP 5973	US80221400	1998	New
	Hewlett-Packard	HP 5975	US61633479	2007	New
	Hewlett-Packard	HP 5973	US00023149	1999	New
	Hewlett-Packard	HP 5973	US00023182	1999	New
	Varian	Saturn 2200	06370 13651 CP8400-6358	2007	New
Volatiles	Hewlett-Packard	HP 5973	US800020780	1998	New
	Hewlett-Packard	HP 5973	US10227041	2002	New
	Hewlett-Packard	HP 5973	US10214090	2002	New
	Hewlett-Packard	HP 5973	US53931405	2005	New

Instrument Type	Manufacturer	Model Number	Serial Number	Year Put Into Service	Condition When Received
General Chemistry	OI Corp	Flow System	20850488	2000	New
	Systea	EasyChem Plus	2006E1001205	2006	New
	Man-Tech Associates	PC-Titrate	190H0238 2330 MS-0L0-477 MS-0C1-471 MS-0B1-276 MS-0E1-579	2001	New
	Mettler-Toledo S/N	MC126 / 225646	225646	2004	New
	Dionex	DX500	99120668	1999	New
	Dionex	ICS-2000	3040054	2003	New
	Dionex	ICS-1000	4010013	2004	New
	Accumet	AB15	AB92321437	2005	New
	Thermo	Genesis 20	3SGH080004	2005	New
	OI Corp	Model 1010 Solids Module	J245710347 C247776181	2003	New
	HF Scientific	Micro 100	402223	2004	New

**Table 21-2 Example: Schedule of Routine Maintenance**

INSTRUMENT	MAINTENANCE	FREQUENCY
APCI/ESI LC/MS/MS	Change pump seals. Change in-line filters in autosampler (HPLC). Check/replace in-line frit if excessive pressure or poor performance. Replace column if no change following in-line frit change. Clean corona needle. Replace sample inlet tube in APCI (10.1 cm). Replace fused silica tube in ESI interface. Clean lenses. Clean skimmer. Ballast rough pump 30 minutes.	As Needed
	Check solvent reservoirs for sufficient level of solvent. Verify that pump is primed, operating pulse free. Check needle wash reservoir for sufficient solvent. Verify capillary heater temperature. Verify vaporizer heater temperature. Verify rough pump and turbo-pump oil levels. Verify nitrogen pressure for auxiliary and sheath gasses. Verify that corona and multiplier are functioning.	Daily <sup>(2)</sup>
	Replace rough-pump oil (4-6 months). Vacuum/clean inlet foam. Replace oil mist filter. Replace activated alumina filter.	Semi-Annually
	Vacuum system components including fans and fan covers.	Annually
HIGH PRESSURE LIQUID CHROMATOGRAPH(1)	Replace columns when peak shape and resolution indicate that chromatographic performance of column is below method requirements. Rinse flow cell with 1N nitric acid if dirty flow cell. Change pump seals when flow becomes inconsistent. Backflush column if applicable. Change in-line filters for solvents.	As Needed
	Check level of solution in reservoirs. If adding, verify that solvent is from the same source. If changing, rinse gas and delivery lines to prevent contamination of the new solvent. Check gas supply if applicable. Flush with an appropriate solvent to remove all bubbles. Pre-filter all samples.	Daily <sup>(2)</sup>
	Change pump seals.	Every 6-9 Months

INSTRUMENT	MAINTENANCE	FREQUENCY
GAS CHROMATOGRAPH(1)	Replace septum. Clean injector port Break off front portion of capillary columns. Replace column if this fails to restore column performance or when column performance (e.g. peak tailing, poor resolution, high backgrounds, etc.) indicates it is required. Change glass wool plug in injection port and/or replace injection port liner when front portion of capillary column is removed. Perform gas purity check (if high baseline indicates that impure carrier gas may be in use). Replace or repair flow controller if constant gas flow cannot be maintained. Detectors: clean when baseline indicates contamination or when response is low. FID: clean/replace jet, replace ignitor. PID: clean lamp window or replace as needed, replace seals. ECD: follow manufacturers suggested maintenance schedule Replace fuse. Reactivate external carrier gas dryers. HP 7673 Autosampler: replace syringe, fill wash bottle, dispose of waste bottle contents. Check inlets, septa.	As Needed
	Check for sufficient supply of carrier and detector gases. Check for correct column flow and/or inlet pressures. Check temperatures of injectors and detectors. Verify temperature programs. Check baseline level. Inspect chromatogram to verify symmetrical peak shape and adequate resolution between closely eluting peaks.	Daily <sup>(2)</sup>
	ECD: perform wipe test.	Semi-Annually
PURGE AND TRAP SYSTEMS	Change trap. Check purge flow. Flush lines (after foaming sample). Periodic leak checks quarterly, replace/condition traps (when poor response or disappearance of reactive or poorly trapped compounds), clean sample lines, valves (if they become contaminated), and clean glassware. Check purge flow. Bake trap as needed to correct for high background. Change trap whenever loss of sensitivity, or erratic response or failing resolution is observed. Purge & trap autosamplers: leak check system, clean sample lines, valves.	As Needed
	Bake out trap prior to commencing analysis.	Daily <sup>(2)</sup>
GAS CHROMATOGRAPHY/LOW-RESOLUTION MASS SPECTROMETER <sup>(1)</sup>	Replace septum. Clean injector port. Break off front portion of capillary columns. Replace column if this fails to restore column performance or when column performance (e.g. peak tailing, poor resolution, high backgrounds, etc.) indicates it is required. Replace injection port liner when front portion of capillary column is removed. Check level of oil in mechanical pumps and diffusion pump	As Needed

INSTRUMENT	MAINTENANCE	FREQUENCY
	<p>if vacuum is insufficient. Add oil if needed.  Replace electron multiplier when the tuning voltage approaches the maximum and/or when sensitivity falls below required levels.  Clean Source, including all ceramics and lenses - the source cleaning is indicated by a variety of symptoms including inability of the analyst to tune the instrument to specifications, poor response, and high background contamination.  Repair/replace jet separator.  Replace filaments when both filaments burn out or performance indicates need for replacement.  Check mass calibration (PFTBA or FC-43).  Check ion source and analyzer (clean, replace parts as needed).  Check vacuum, relays, gas pressures and flows.  Change oil in the mechanical rough pump.  Relubricate the turbomolecular pump-bearing wick.  HP 7673 Autosampler: Replace syringe.</p>	
	<p>Check for sufficient gas supply. Check for correct column flow and/or inlet pressure.  Check temperatures of injector, detector.  Verify temperature programs.  Check inlets, septa.  Check baseline level.  Check values of lens voltages, electron multiplier, and relative abundance and mass assignments of the calibration compounds.  Inspect chromatogram to verify symmetrical peak shape and adequate resolution between closely eluting peaks.  HP 7673 Autosampler: fill wash bottle, dispose of waste bottle contents.</p>	Daily <sup>(2)</sup>
	<p>Replace the exhaust filters on the mechanical rough pump every 1-2 years.</p>	Annually
<p><b>GAS CHROMATOGRAPHY/HIGH-RESOLUTION MASS SPECTROMETER<sup>(1)</sup></b></p>	<p>Full Bake-Out.  Change oil in rotary pump.  Change oil in diffusion pump. Replace o-rings.  Solvent rinse the flight tube.  Clean the first field free region.  Check the data system ventilation (fans and filters).  Check detector voltages.  Clean and dust connectors, etc on the outside of the instrument.  Check the vacuum: <math>5 \times 10^{-8}</math> MBAR on both analyzer ion gauges, and <math>5 \times 10^{-7}</math> MBAR on the source, with no helium flowing.  Check isolation valve for leaks, correct if needed.  Check for thermal trip by taking the magnet to maximum current, and verify that the coolant flow is acceptable.  Replace septum.  Clean injector port.  Break off front portion of capillary columns. Replace column if this fails to restore column performance or when column performance (e.g. peak tailing, poor resolution, high backgrounds, etc.) indicates it is required.  Change glass wool plug in injection port and/or replace injection port liner when front portion of capillary column</p>	As Needed

INSTRUMENT	MAINTENANCE	FREQUENCY
	<p>is removed.</p> <p>Clean Source, including all ceramics and lenses - the source cleaning is indicated by a variety of symptoms including inability of the analyst to tune the instrument to specifications, poor response, and high background contamination.</p> <p>Repair/replace jet separator.</p> <p>Replace filaments when both filaments burn out or performance indicates need for replacement.</p>	
	<p>Check resolution sensitivity.</p> <p>Check stability.</p> <p>Check for sufficient gas supply. Check for correct column flow and/or inlet pressure.</p> <p>Check temperatures of injector, detector.</p> <p>Verify temperature programs.</p> <p>Check inlets, septa.</p> <p>Check baseline level.</p> <p>Check values of lens voltages, electron multiplier, and relative abundance and mass assignments of the calibration compounds.</p> <p>Inspect chromatogram to verify symmetrical peak shape and adequate resolution between closely eluting peaks.</p>	Daily <sup>(2)</sup>
COLD VAPOR ATOMIC ABSORPTION (LEEMAN PS 200) <sup>(1)</sup>	<p>Change pump tubing.</p> <p>Check/change Hg lamp.</p> <p>Clean optical cell.</p> <p>Change drying tube.</p> <p>Grease pump.</p>	As Needed
	<p>Check sample tip for clogs.</p> <p>Check drying tube.</p> <p>Check pump tubing/drain tubing.</p> <p>Check gas pressure.</p> <p>Check liquid/gas separator.</p> <p>Check tubing.</p>	Daily <sup>(2)</sup>
INDUCTIVELY COUPLED ARGON PLASMA/MASS SPECTROMETRY (ICAP/MS) <sup>(1)</sup>	<p>Check electronic settings for optimum sensitivity: resolution, mass calibration, ion optics.</p> <p>Measure quartz torch for proper alignment when removed and cleaned.</p> <p>Clean spray chamber and nebulizer.</p> <p>Clean all filters and fans.</p> <p>Check chiller coolant level.</p> <p>Check and drain oil mist eliminator on roughing pumps.</p>	As Needed
	<p>Check sample waste container level.</p> <p>Check quartz torch condition.</p> <p>Check RF coil.</p> <p>Check peristaltic pump: proper roller pressure, sample introduction tubing, correct pump rotation, condition of drain tubing.</p> <p>Check condition of sampler and skimmer cones.</p> <p>Check oil level of roughing pumps.</p>	Daily <sup>(2)</sup>
	<p>Replace oil in roughing pumps.</p>	Every 2-3 Months
ICP <sup>(1)</sup>	<p>Check that argon feed pressure is 80-120 psi.</p> <p>Check that chiller coolant pressure is 45-80 psig, no leaks.</p> <p>Check purge and shear gasses. Nitrogen purge gas pressure 40-120 psig, compressed air shear gas pressure 80-120 psig.</p> <p>Check radial purge and axial windows for deposits.</p> <p>Check that nebulizer is not clogged.</p> <p>Check that capillary tubing is clean and in good condition.</p>	Daily <sup>(2)</sup>

INSTRUMENT	MAINTENANCE	FREQUENCY
	Check that peristaltic pump windings are secure. Check that exhaust vent is operational Check that torch, glassware, aerosol injector tube are clean.	
	Clean plasma torch assembly to remove accumulated deposits. Check RF coil. Clean nebulizer and drain chamber; keep free flowing to maintain optimum performance. Clean filters on back of power unit to remove dust. Replace when needed: peristaltic pump tubing. sample capillary tubing. autosampler sipper probe. Check performance with yttrium or sodium. Check O-rings. Clean/lubricate pump rollers	Monthly or As Needed
	Check chiller coolant filter. (may require more or less frequently)	Semi-Annually
	Notify manufacturer service engineer for scheduled preventive maintenance service.	Annually
ION CHROMATOGRAPH <sup>(1)</sup>	Clean micromembrane suppressor when decreases in sensitivity are observed. Check fuses when power problems occur. Change column when peak shape and resolution deteriorate or when retention time shortening indicates that exchange sites have become deactivated. De-gas pump head when flow is erratic. Check all air and liquid lines for discoloration and crimping, if indicated. Check/change bed supports guard and analytical columns, if indicated.	<b>As Needed</b>
	Check plumbing/leaks. Check gases. Check pump pressure. Check conductivity meter.	Daily <sup>(2)</sup>
	Check pump heads for leaks. Check filter (inlet).	Weekly
	Change pump seals. Change injection valve. Clean conductivity cell. Check conductivity cell for calibration.	Annually
ALPKEM COLORIMETRIC AUTO ANALYZER <sup>(1)</sup>	Prepare fresh reagents. Replace tubing. (About every 100 hours of use)	As Needed
	Check detector. Make sure there are no trapped bubbles in detector cell. Check Valves Check peristaltic tubing. Check sampler. Check auto diluter.	Daily <sup>(2)</sup>
	Clean pump, diluter, and XYZ Sampler.	Weekly
	Lubricate pump roller.	Monthly
	Clean pump rollers with steel wool and lubricate.	Semi-Annually
CHEMICAL OXYGEN DEMAND (COD) REACTOR <sup>(1)</sup>	Electronics serviced.	<b>As Needed</b>

INSTRUMENT	MAINTENANCE	FREQUENCY
	Check temperature with NIST reference thermometer.	Annually
AUTO TITRATOR <sup>(1)</sup>	Electronics serviced.	As Needed
	Calibrate with check standards. Inspect electrodes daily, clean as needed. Inspect electrode proper levels of filling solutions daily, fill as needed. Clean probe, each use. Prime buret Check rinse water reservoir.	Daily <sup>(2)</sup> (When Used)
CONDUCTANCE METER <sup>(1)</sup>	Electronics serviced. Replace batteries	As Needed
SPECTROPHOTOMETER <sup>(1)</sup>	Check probe and cables. Check calibration. Inspect conductivity cell	Daily <sup>(2)</sup> (When Used)
	Replace lamp. Replace fuse.	As Needed
	Check instrument manual. Perform wavelength calibration. Replace lamp annually or when erratic response is observed.	Annually
PH METER <sup>(1)</sup>	Clean electrode. Refill reference electrode.	As Needed
	Inspect electrode. Verify electrodes are properly connected and filled. Inspect electrode proper levels of filling solutions. Make sure electrode is stored in buffer.	Daily <sup>(2)</sup>
TOTAL ORGANIC CARBON ANALYZER (OI 1010 AND SOLIDS)	Check injection port septum after 50-200 runs. Perform leak test. Calibrate reagent pumps. Change sample loops. Adjust flow. Indicating drying tube. NDIR zero, after 100 hours of use. Sample pump, after 2000 hours for use. Digestion vessel/condensation chamber. Permeation tube, after 2000 hours of use. NDIR cell, after 2000 hours of use.	As Needed
	Check: Oxygen supply, (nitrogen supply for solids). Persulfate supply (1010 unit). Acid supply (1010 unit). Rinse water reservoir supply (1010 unit). IR millivolts for stability (after 30 min. warm-up).	Daily <sup>(2)</sup>
TURBIDIMETER <sup>(1)</sup>	Electronics serviced.	As Needed
	Adjust linearity on varying levels of NTU standards. Standardize with NTU standards. Inspect cells.	Daily <sup>(2)</sup> (When Used)
	Clean instrument housing.	Monthly
DIGESTION BLOCK	Check temperature with NIST thermometer.	Annually
SONICATOR <sup>(1)</sup>	Replace probe tip. Disassemble and clean sonicator probe tips. Tune sonicator assembly.	As Needed
	Inspect probe tips for inconsistencies (etching/pitting).	Daily <sup>(2)</sup> (When Used)
ANALYTICAL/TOP LOADING BALANCES <sup>(1)</sup>	Check using ASTM Class 3 weights once daily or before use. Clean pan and weighing compartment.	Daily <sup>(2)</sup>

INSTRUMENT	MAINTENANCE	FREQUENCY
REFRIGERATORS/WALK-IN COOLERS <sup>(1)</sup>	Manufacturer cleaning and calibration.	Annually
	Refrigerant system and electronics serviced.	As Needed
	Temperatures checked and logged.	Daily <sup>(2)</sup>
OVENS <sup>(1)</sup>	Electronics serviced.	<b>As Needed</b>
	Temperatures checked and logged.	Daily <sup>(2)</sup>
ZYMARK PE WORKSTATION	<p>Change O-rings whenever there are visible leaks or poor sealing on the SPE columns.</p> <p>Sample lines are clean after samples have been extracted by SPE with a program "Clean Sample Lines" with methanol followed by water. Occasionally for a more rigorous cleaning, or after a highly contaminated sample, a mixture of methanol/DCM at 50:50 may be used in place of methanol, follow by methanol, then water (never use acetone).</p> <p>Syringe pump may be primed using a program "Prime Solvent Lines" whenever air bubbles are suspected in the lines from running out of solvents and whenever solvents are changed.</p> <p>Syringe pump in good condition – replace if showing signs of wear or suspected of poor performance.</p> <p>Sample pumps may be re-calibrated whenever major repairs are performed, or whenever the pumps are suspected to be out of calibration. Follow manufacturer's procedure for re-calibrating the sample pumps. For method 8330, the pump loads 1050 mL of sample on the SPE. It should used up the whole sample bottle (quart bottles and 1-L bottles).</p>	<b>As Needed</b>
SONICATION WATER BATH <sup>(1)</sup>	<p>If the water bath is dirty, empty and refill with tap water. A couple drops of anti-bacterial solution may be added to inhibit the growth of bacteria in the water.</p> <p>The water level in the sonication batch should be about 1.2 to 1 inch from the top while in operation. Do not allow sonication batch to operate with water bath at lower levels. If the level is low, add more water, if the levels is too high, remove water to the proper level.</p>	As Needed
RECIRCULATING COOLER <sup>(1)</sup>	<p>Check the water level in the recirculating cooler – the water level should be about ½ inch from the top while in operation. If the level is low, add more distilled water to the proper level. A couple drops of anti-bacterial solution may be added to inhibit the growth of bacteria in the water.</p> <p>Check the conditions on the tubing to and from the recirculating cooler, and the clamps on the tubing. Replace if they are showing signs of wear or are worn or broken.</p>	As Needed

**Footnotes to Preventive Maintenance Tables**

- (1) Refer to manufacturer's instructions for each instrument to identify and perform maintenance operations.
- (2) Daily checks and verifications are performed prior to instrument startup and are not documented in maintenance logs unless problems are noted.

**Table 21-3.**

**Example: Periodic Calibration**

<b>Instrument</b>	<b>Type of Calibration/ Number of Standards</b>	<b>Frequency</b>	<b>Acceptance Limits</b>	<b>Corrective Action</b>
Analytical Balance	Accuracy determined using A2LA-accredited NIST weights.  Minimum of 2 standards bracketing the weight of interest.  Inspected and calibrated by A2LA accredited person annually. A second annual inspection and calibration by same firm.	Daily	± 0.2%	Clean, check level, insure lack of drafts, and that unit is warmed up, recheck. If fails, call service.
Top Loading Balance	Accuracy determined using A2LA-accredited NIST weights.  Minimum of 2 standards bracketing the weight of interest.  Inspected and calibrated by A2LA accredited person annually. A second annual inspection and calibration by same firm.	Daily	± 0.5%	Clean. Replace.
A2LA-accredited NIST Weights	Accuracy determined by accredited weights and measurement laboratory.	1 year	As per certificate.	Replace.
NIST-Traceable Thermometer	Accuracy determined by A2LA-accredited weights and measurement laboratory.	5 years	As per certificate.	Replace.
Thermometer	Against NIST-traceable thermometer	Yearly at appropriate temperature range for intended use	± 1.2°C	Replace.
Minimum-Maximum Thermometers	Against NIST-traceable thermometer	Yearly	± 1.5°C	Replace.

<b>Instrument</b>	<b>Type of Calibration/ Number of Standards</b>	<b>Frequency</b>	<b>Acceptance Limits</b>	<b>Corrective Action</b>
Infrared Temperature Guns	Against NIST-traceable thermometer	Quarterly at appropriate temperature range for intended use.	$\pm 1.5^{\circ}\text{C}$	Repair/replace.
Dial-type Thermometers	Against NIST-traceable thermometer	Quarterly at appropriate temperature range for intended use.	$\pm 1.5^{\circ}\text{C}$	Replace.
Refrigerator	Temperature checked using NIST-traceable thermometer.	Daily. If out of range, check again in two hours.	$2.7 \pm 1.7^{\circ}\text{C}$	Adjust. Repair. While waiting for repair, seal door, attach "Out of Service" sign, move items to functional unit. Notify supervisor.
Freezer	Temperature checked using NIST-traceable thermometer	Daily. If out of range, check again in two hours.	$(-10)-(-20)^{\circ}\text{C}$	Adjust. Repair. While waiting for repair, seal door, attach "Out of Service" sign, move items to functional unit. Notify supervisor.
Oven	Temperature checked using NIST-traceable thermometer.	When in use.	$104 \pm 1^{\circ}\text{C}$ (drying) $180 \pm 2^{\circ}\text{C}$ (TDS)	Adjust. Replace.
Water Bath	Temperature checked using NIST-traceable thermometer.	When in use.	$\pm 2^{\circ}\text{C}$	Adjust. Replace.
Volumetric Dispensing Devices (Eppendorf® pipette, automatic dilutor or dispensing devices)	One delivery by weight. Using DI water, dispense into tared vessel. Record weight with device ID number.	Monthly	$\pm 2\%$ Calculate accuracy by dividing weight by stated volume times 100 for percent.	Adjust. Replace.
Glass Microliter Syringes	None	Accuracy must be initially demonstrated if syringe was not received with a certificate attesting to established accuracy.	$\pm 1\%$	Not applicable.

<b>Instrument</b>	<b>Type of Calibration/ Number of Standards</b>	<b>Frequency</b>	<b>Acceptance Limits</b>	<b>Corrective Action</b>
Conductivity Meter	Cell impedance calibrated with three KCl standards.	Each use.	$r \geq 0.99$	Recalibrate.
Deionized Water	Check in-line conductivity meter on system with conductivity meter in Inorganics Department.	Weekly	$<10 \mu\text{mhos}/\text{cm}^2$	Record on log. Report discrepancies to QA Director.

## SECTION 22

### MEASUREMENT TRACEABILITY (NELAC 5.5.6)

#### 22.1 OVERVIEW

Traceability of measurements shall be assured using a system of documentation, calibration, and analysis of reference standards. Laboratory equipment that are peripheral to analysis and for which calibration is not necessarily documented in a test method analysis or by analysis of a reference standard shall be subject to ongoing certifications of accuracy. At a minimum, these must include procedures for checking specifications of ancillary equipment: balances, thermometers, temperature, Deionized (DI) and Reverse Osmosis (RO) water systems, automatic pipettes and other volumetric measuring devices. With the exception of Class A Glassware (including glass microliter syringes that have a certificate of accuracy), quarterly accuracy checks are performed for all mechanical volumetric devices. Wherever possible, subsidiary or peripheral equipment is checked against standard equipment or standards that are traceable to national or international standards. The following definitions are provided by the American Association for Laboratory Accreditation (A2LA):

“Traceability is the property of a measurement result whereby it can be related to stated references, usually national or international standards, through an unbroken chain of comparisons, each step in the chain having stated uncertainties.” There are six essential elements:

- An unbroken chain of comparison
- A calculated measurement uncertainty for each step in the chain to allow for an overall uncertainty calculation
- Documentation of each step in each calibration report
- All steps in the chain are performed by individuals with evidence of technical competence and accredited by a recognized accreditation body
- Reference to International Standard (SI) units
- Recalibration at appropriate intervals to preserve traceability

Calibration is defined as “determining and documenting the deviation of the indication of a measuring instrument (or the stated value of a material measure) from the conventional ‘true’ value of the measurand.”

Uncertainty is defined as “a parameter associated with the result of a measurement that characterizes the dispersion of the value that could reasonably be attributed to the measurand.” Measurement of Uncertainty is discussed in Section 20 of this QA Manual.

## **22.2 NIST-TRACEABLE WEIGHTS AND THERMOMETERS**

Reference standards of measurement shall be used for calibration only and for no other purpose, unless it can be shown that their performance as reference standards would not be invalidated.

For NIST-traceable weights and thermometers, the laboratory requires that all calibrations be conducted by a calibration laboratory accredited by A2LA, NVLAP (National Voluntary Laboratory Accreditation Program), APLAC (Asia-Pacific Laboratory Accreditation Cooperation), or EA (European Cooperation for Accreditation). A certificate and scope of accreditation is kept on file at the laboratory. Refer to Section 21 for calibration of weights and thermometers.

## **22.3 REFERENCE STANDARDS / MATERIALS**

Reference standards/materials, where commercially available, are traceable to certified reference materials. Commercially prepared standard materials are purchased from vendors accredited by A2LA, or NVLAP with an accompanying Certificate of Analysis that documents the standard purity. If a standard cannot be purchased from a vendor that supplies a Certificate of Analysis, the purity of the standard is documented by analysis. (Refer to Section 9 for additional information on purchasing). The receipt of all reference standards must be documented. Reference standards are labeled with a unique Standard Identification Number and expiration date. All documentation received with the reference standard is retained as a QC record and references the Standard Identification Number.

All reference, primary and working standards/materials, whether commercially purchased or laboratory prepared, must be checked regularly to ensure that the variability of the standard or material from the 'true' value does not exceed method requirements. The accuracy of calibration standards is checked by comparison with a standard from a second source. In cases where a second standard manufacturer is not available, a vendor certified different lot is acceptable for use as a second source. For unique situations, such as air analysis where no other source or lot is available, a standard made by a different analyst would be considered a second source. The appropriate Quality Control (QC) criteria for specific standards are defined in laboratory SOPs. In most cases, the analysis of an Initial Calibration Verification (ICV) or LCS (where there is no sample preparation) is used as the second source confirmation. These checks are generally performed as an integral part of the analysis method (e.g. calibration checks, laboratory control samples).

All standards and materials must be stored and handled according to method or manufacturer's requirements in order to prevent contamination or deterioration. Refer to Table 9-1 in Section 9 for general storage requirements and Table 22-1 for additional storage information. Please refer to method SOPs "Standards and Reagents" section for additional details. For safety requirements, please refer to method SOPs and the laboratory Environmental Health and Safety Manual.

## **22.4 DOCUMENTATION AND LABELING OF STANDARDS, REAGENTS, AND REFERENCE MATERIALS**

Reagents must be at a minimum the purity required in the test method. The date of reagent receipt and the expiration date are documented. The lots for most of the common solvents and

acids are tested for acceptability prior to company wide purchase. Refer to SOP No. CA-Q-S-001, "Solvent and Acid Lot Testing and Approval".

All manufacturer or vendor supplied Certificate of Analysis or Purity must be retained, stored appropriately, and readily available for use and inspection. These records are maintained in scanned files on the network, or in binders in the department. Records must be kept of the date of receipt and date of expiration of standards, reagents and reference materials. In addition, records of preparation of laboratory standards, reagents, and reference materials must be retained, stored appropriately, and be readily available for use and inspection. For detailed information on documentation and labeling, please refer to SOP No. WS-QA-0017, "Standards and Reagent Preparation and Quality Control Check Procedures".

Commercial materials purchased for preparation of calibration solutions, spike solutions, etc., are usually accompanied with an assay certificate or the purity is noted on the label. If the assay purity is 96% or better, the weight provided by the vendor may be used without correction. If the assay purity is less than 96% a correction will be made to concentrations applied to solutions prepared from the stock commercial material (for 1613B dioxin/furan analyses the purity must be 98% or corrections must be made).

**22.4.1** All standards, reagents, and reference materials must be labeled in an unambiguous manner. Standards are logged into the laboratory's standard logbook program or into hardcopy standards logbook, and are assigned a unique identification number. The following information is typically recorded in the electronic database or standards logbook:

- Standard ID
- Description of Standard
- Preparer's name
- Final volume and number of vials prepared
- Solvent type and lot number
- Preparation Date
- Expiration Date
- Standard source type (stock or daughter)
- Standard type (spike, surrogate, other)
- Parent standard ID (if applicable)
- Parent Standard Analyte Concentration (if applicable)
- Parent Standard Amount used (if applicable)
- Component Analytes
- Final concentration of each analyte
- Comment box (text field)

Records are maintained electronically for standard and reference material preparation for most departments. These records show the traceability to purchased stocks or neat compounds.

These records also include method of preparation, date of preparation, expiration date and preparer's name or initials. Preparation procedures are provided in the Method SOPs.

**22.4.2** All standards, reagents, and reference materials must be clearly labeled with a minimum of the following information:

- Expiration Date
- Standard ID
- Special Health/Safety warnings if applicable (refer to the method SOP for specifics)
- Reagent Preparation Date (if applicable)

**22.4.3** In addition, the following information may be helpful:

- Date of receipt for commercially purchased items or date of preparation for laboratory prepared items
- Date opened (for multi-use containers, if applicable)
- Description of standard (if different from manufacturer's label or if standard was prepared in the laboratory)
- Concentration (if applicable)
- Initials of analyst preparing standard or opening container

All containers of prepared reagents must include a preparation date, expiration date and an ID number to trace back to preparation.

Procedures for preparation of reagents can be found in the Method SOPs.

Standard ID numbers must be traceable through associated logbooks, worksheets and raw data.

All reagents and standards must be stored in accordance to the following priority: 1) with the manufacturer's recommendations; 2) with requirements in the specific analytical methods; and 3) according to method SOPs.

## **SECTION 23.0**

### **SAMPLING (NELAC 5.5.7)**

#### **23.1 OVERVIEW**

TestAmerica West Sacramento does not provide sampling services. The laboratory's responsibility in the sample collection process lies in supplying the sampler with the necessary coolers, reagent water, sample containers, preservatives, sample labels, custody seals, COC forms, ice, and packing materials required to properly preserve, pack, and ship samples to the laboratory

#### **23.2 SAMPLING CONTAINERS**

The laboratory offers clean sampling containers for use by clients. These containers are obtained from reputable container manufacturers and meet EPA specifications as required. Any certificates of cleanliness that are provided by the supplier are maintained at the laboratory.

##### **23.2.1 Preservatives**

Upon request, preservatives are provided to the client in pre-cleaned sampling containers. In some cases containers may be purchased pre-preserved from the container supplier. Whether prepared by the laboratory or bought pre-preserved, the grades of the preservatives are at a minimum:

- Hydrochloric Acid – Reagent ACS (Certified VOA Free) or equivalent
- Methanol – Purge and Trap grade
- Nitric Acid – Instra-Analyzed or equivalent
- Sodium Bisulfate – ACS Grade or equivalent
- Sodium Hydroxide – Instra-Analyzed or equivalent
- Sulfuric Acid – Instra-Analyzed or equivalent
- Sodium Thiosulfate – ACS Grade or equivalent

##### **23.2.2 Preparing Container Orders**

When new containers arrive at the laboratory, the date of receipt is recorded on the packing list received with them for retained documentation. Upon request, the containers are then sent to clients for use in collecting samples. The shipping date, type and number of containers are maintained on file by the lab. Shipping personnel insure that container stock is rotated so that "first in" is "first out." When a client requests containers, a client services representative creates a container request in a database program; it is then stored permanently in the program with a unique container order number. Copies of the container request are printed for the shipping department. One copy goes to the client with the containers. Refer to SOP No. SAC-QA-0007, "Bottle and Cooler Preparation".

The laboratory also provides EnCore, TerraCore or other soil sampling devices when requested.

If containers are provided directly to the client from the manufacturer or from other sources, the laboratory will not be responsible for any of the above records.

### **23.3 FIELD QUALITY CONTROL (QC)**

Common field quality control samples are defined in the following paragraphs. The frequency of field quality control samples should be specified in the site specific Quality Assurance Project Plan (QAPP) or by the client. TestAmerica provides trip blanks for VOC analysis with the sample containers for all volatile organic analyses. Blanks generated in the field will be analyzed along with the field samples (exception soil samples where the blank is aqueous).

**23.3.1 Equipment Blank / Rinsate Blank** - The equipment blank, sometimes referred to as a rinsate blank, is a sample of the water used to decontaminate sampling equipment. The source water should be as free of target analytes as possible. An aliquot of this water is poured over or through the sample collection device after decontamination, collected in a sample container, preserved with appropriate reagents, and returned to the laboratory. This serves as a check on sampling device cleanliness, and will also be affected by the site and sample handling conditions evaluated by the other types of blanks. The sampling time for the equipment blank should begin when the equipment is rinsed and the water is collected.

**23.3.2 Field Blank** - The field blank is water that is as free of target analytes as possible and from the same source as the equipment blank. The water is poured into a sampling container at the sampling site, preserved with the appropriate reagents, and returned to the laboratory. This serves as a check on reagent and environmental contamination. The sampling time for the field blank should be when the blank is prepared in the field.

**23.3.3 Trip Blank** - The trip blank pertains to volatile analysis only. This serves as a check on sample contamination originating from sample transport, sample container contamination, shipping and storage, or from certain site conditions. Trip blanks are often referred to as travel blanks. They are prepared using pre-cleaned sample containers. They are filled with organic-free water (the source of the organic free water is the same source of water used to prepare volatile standards, method blanks, LCS and sample dilutions), sealed and taken into the field with the empty containers which will be used for sampling. The recommended frequency is one trip blank per cooler (in duplicate or triplicate), per volatiles method. Unless otherwise specified, the sampling time for the trip blank is the time of receipt at the laboratory (When the "Trip" ends).

**23.3.4 Field Duplicates** - Field duplicates are replicate samples collected from the same sampling point or location during a field collection event. This control sample is used to demonstrate the ability of both the sampling and analytical process to generate data of acceptable precision.

### **23.4 DEFINITION OF HOLDING TIME**

The date and time of sampling documented on the chain-of-custody (COC) form establishes the day and time zero. As a general rule, when the maximum allowable holding time is expressed in "days" (e.g. 14 days, 28 days), the holding time is based on calendar day measured. Holding

times expressed in “hours” (e.g. 6 hours, 24 hours, etc.) are measured from date and time zero. The first day of holding time ends twenty-four hours after sampling. Holding times for analysis include any necessary reanalysis. However there are some programs, such as AFCEE and Alaska Department of Environmental Conservation, that determine holding time compliance based on the date and specific time of analysis compared to the time of sampling regardless of how long the holding time is.

**23.4.1** Semi-Volatile - Holding times for sample preparation for semi-volatile organics are measured from the sampling date (and time where applicable) until the day (and time where applicable) solvent contacts the sample. If a sample is to be extracted on the day of expiration, the actual time of extraction must be recorded on the sample preparation worksheet. Holding times for analysis are measured from the date (and time where applicable) of initiation of extraction to the time of injection into the gas chromatograph.

**23.4.2** Volatiles - Holding times for volatile organics are measured from the date (and time where applicable) of sampling to the date and time of injection into the gas chromatograph. The time of initiation of purging is considered the injection time, but data systems record the start of the chromatographic run rather than the start of purging. Hence, if a sample is so near expiration that the start-of-purging time rather than the chromatographic run time is needed to document the integrity of the sample; the analyst must observe and record the start-of-purging time in the instrument log. Extractions, e.g. for high level soils, must be completed in time to allow for analysis to be initiated within the maximum allowable holding time.

**23.4.3** Inorganics - For inorganic and metals analysis, the preparation/digestion/distillation must be started within the maximum holding time as measured from the sampling date (and time where applicable).

## **23.5** SAMPLING CONTAINERS, PRESERVATION REQUIREMENTS, HOLDING TIMES

The preservation and holding time criteria specified in the following tables are derived from the source documents for the methods. If method required holding times (refer to Tables 23-1 to 23-7) or preservation requirements are not met, the reports will be qualified using a flag, footnote or case narrative. As soon as possible or “ASAP” is an EPA designation for tests for which rapid analysis is advised, but for which neither EPA nor the laboratory have a basis for a holding time.

## **23.6** SAMPLE ALIQUOTS / SUBSAMPLING

Taking a representative sub-sample from a container is necessary to ensure that the analytical results are representative of the sample collected in the field. The size of the sample container, the quantity of sample fitted within the container, and the homogeneity of the sample need consideration when sub-sampling for sample preparation. It is the laboratory’s responsibility to take a representative subsample or aliquot of the sample provided for analysis. In that regard the following guidelines apply to analysts:

Analysts should handle each sample as if it is potentially dangerous. At a minimum, safety glasses, gloves, and lab coats must be worn when preparing aliquots for analysis.

Refer to SOP Nos. WS-QA-0018, "Subsampling and Compositing of Samples (Method ASTM D 6323-98)" and WS-QA-0028, "Multi-Incremental Subsampling of Soils and Sediments" for subsampling details.

Tables 23-1 to 23-7 detail holding times, preservation and container requirements, and sample volumes for SDWA and NPDES methods. The sample volumes are intended to be a minimal amount to perform the method, the containers that are used may be of larger size. **Please Note:** *The holding times are program specific and different programs may have different holding times for equivalent methods (e.g., there are differences in Holding times for many Organic analytes between SDWA and NPDES. RCRA methods may also be different.)*

**Table 23-1.  
Holding Times, Preservation and Container Requirements: Drinking Water (SDWA)**

PARAMETER	CONTAINER	PRESERVATION <sup>1,2</sup>		HOLDING TIME <sup>3</sup>	SAMPLE VOLUME
		Temp. <sup>23</sup>	Chemical		
Asbestos	Plastic/Glass	4°C	None	48 hours <sup>5</sup>	1 L
Coliforms (Total and Fecal)	Plastic/Glass <sup>20</sup>	10°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	30 hours <sup>21</sup>	120 mL
Cyanide	Plastic/Glass	4°C	NaOH to pH >12 Ascorbic acid <sup>9</sup> or Sodium arsenite <sup>9</sup>	14 days	500 mL
Fluoride	Plastic/Glass	None	None	None	250 mL
Heterotrophic Plate Count	Plastic/Glass <sup>20</sup>	10°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	8 hours (24 hours <sup>22</sup> )	120 mL
Mercury	Plastic/Glass	None	HNO <sub>3</sub> to pH<2	28 days	250 mL
Metals <sup>4</sup>	Plastic/Glass	None	HNO <sub>3</sub> to pH<2 <sup>24</sup>	6 months	250 mL
Nitrate	Plastic/Glass	4°C	None	48 hours <sup>6</sup>	250 mL
Nitrate-Nitrite	Plastic/Glass	None	H <sub>2</sub> SO <sub>4</sub> to pH<2	28 days	250 mL
Nitrite	Plastic/Glass	4°C	None	48 hours	250 mL
THMs Only	Glass <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>9</sup> HCl to pH <2 may also be used	14 days	3 X 40 mL
Volatile Organic Compounds	Glass <sup>8</sup>	4°C	HCl to pH <2 Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>9</sup> or Ascorbic acid <sup>9</sup>	14 days	3 X 40 mL
EDB, DBCP, 1,2,3- TCP (EPA 504.1)	Glass <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	14 days	3 X 40 mL
Organochlorine Pesticides/PCBs (EPA 505) <sup>10</sup>	Glass <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	14 days <sup>11</sup>	3 X 40 mL
Nitrogen and Phos. Pesticides (EPA 507)	Glass-Amber <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	14 days <sup>12</sup>	1 L
Total PCBs (EPA 508A)	Glass-Amber <sup>8</sup>	4°C	None	14 days <sup>13</sup>	1 L
Pesticides and PCBs (EPA 508.1) <sup>14</sup>	Glass-Amber <sup>8</sup>	4°C	HCl to pH <2 Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>9</sup>	14 days <sup>13</sup>	1 L

PARAMETER	CONTAINER	PRESERVATION <sup>1,2</sup>		HOLDING TIME <sup>3</sup>	SAMPLE VOLUME
		Temp. <sup>23</sup>	Chemical		
Chlorinated Acids (EPA 515.1)	Glass-Amber <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	14 days <sup>12</sup>	1 L
Semivolatiles (EPA 525.2)	Glass-Amber <sup>8</sup>	4°C	HCl to pH <2 Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>9</sup>	14 days <sup>13</sup>	1 L
N-Methylcarbamoyloxamines and N-Methcarbamates (EPA 531.1)	Glass <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> , Monochloroacetic Acid buffer to pH<3	28 days	3 X 60 mL
Glyphosate (EPA 547)	Glass <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	14 days	3 X 60 mL
Endothall (EPA 548)	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	4°C	None	7 days <sup>15</sup>	1 L
Diquat/Parquat (EPA 549.1)	Glass-Amber <sup>8</sup> (Silanized or PVC amber)	4°C	H <sub>2</sub> SO <sub>4</sub> to PH <2 Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>9</sup>	7 days <sup>16</sup>	1 L
Chlorinated Disinfection Byproducts, Chlorinated Solvents, and Halogenated Pesticides/Herbicides (EPA 551)	Glass <sup>8</sup>	4°C	Phosphate Buffer and Ammonium Chloride <sup>19</sup>	14 days <sup>17</sup>	3 X 60 mL
Haloacetic Acids (EPA 552.1)	Glass-Amber <sup>8</sup>	4°C	Ammonium Chloride	28 days <sup>18</sup>	250 mL
2,3, 7, 8 TCDD	Glass-Amber <sup>8</sup>	4°C	Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>	1 year	1 L

**Key to Table**

1. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
2. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO<sub>3</sub>) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H<sub>2</sub>SO<sub>4</sub>) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
3. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
4. All metals except Hg.
5. Instructions for containers, preservation procedures and holding times as specified in Method 100.2 must be adhered to for all compliance analysis including those conducted with Method 100.1.
6. If the sample is chlorinated, the holding time for an un-acidified sample kept at 4°C is extended to 14 days.
7. Nitrate-Nitrite refers to a measurement of total nitrite.

**Key to Table**

8. With Teflon lined septum.
9. If chlorinated, add reagent prior to acidification (for Cyanide, add before NaOH).
10. Heptachlor has a 7 day hold time.
11. 14 days until extraction. 24 hours after extraction.
12. 14 days until extraction. 28 days after extraction.
13. 14 days until extraction. 30 days after extraction.
14. For cyanazine, cool to 4°C only.
15. 7 days until derivitization. 1 day after derivitization.
16. 7 days until extraction. 21 days after extraction.
17. 14 days until extraction. 14 days after extraction.
18. 28 days until extraction. 48 hours after extraction.
19. Sodium Sulfite may be used as a dechlorinating agent in some instances. Verify with laboratory prior to sampling.
20. Sterilized. Plastic must be Polypropylene.
21. 40 CFR part 141.74 regulations to avoid filtration or disinfection state 8 hours (DW compliance testing). Most facilities are using either disinfection or filtration so the 8 would not apply in most cases.
22. 40 CFR part 141.74 regulations for Disinfection By-Product rule state 8 hours (DW compliance testing) where SM 9215 allows up to 24 hours if sample is stored between  $> 0$  and  $\leq 4^{\circ}$  C.
23. For samples with a temperature requirement of 4°C, a sample temperature of just above the water freezing temperature to  $\leq 6^{\circ}$ C is acceptable.
24. Acid preservation may be omitted for shipping and laboratory will acidify at least 24 hours prior to analysis.

**Table 23-2  
Holding Times, Preservation and Container Requirements: NPDES – Bacteria, Protozoa, Toxicity Tests**

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION <sup>2,3</sup>		HOLDING TIME <sup>4</sup>	SAMPLE VOLUME
		Temp.	Chemical		
Total, Fecal, and E.coli Coliforms	Plastic/Glass	10°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>6</sup>	6 hours	100 mL
Fecal Streptococci	Plastic/Glass	10°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>6</sup>	6 hours	100 mL
Enterococci	Plastic/Glass	10°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>6</sup>	6 hours	100 mL
Cryptosporidium	LPDE Plastic	0-8°C	None	96 Hours	500 mL
Giardia	LPDE Plastic	0-8°C	None	96 Hours	500 mL
Toxicity – Acute/Chronic	Plastic/Glass	≤ 6°C <sup>5</sup>	None	36 Hours	2 L

**Key to Table**

1. Plastic should be Polypropylene or other sterilizable plastic.
2. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
3. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO<sub>3</sub>) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H<sub>2</sub>SO<sub>4</sub>) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
4. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
5. Samples must not be frozen. Sufficient ice should be placed with the samples in the shipping container to ensure that ice is still present when the samples arrive at the laboratory. However, even if ice is present, when samples arrive, it is necessary to measure the temperature of the samples and confirm that the ≤ 6°C temperature has not been exceeded.
6. Should only be used in the presence of residual chlorine.

**Table 23-3**  
**Holding Times, Preservation and Container Requirements: NPDES - Inorganic**

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION <sup>2,3</sup>		HOLDING TIME <sup>4</sup>	SAMPLE VOLUME
		Temp <sup>14</sup>	Chemical		
Acidity	Plastic/Glass	≤ 6°C	None	14 days	100 mL
Alkalinity	Plastic/Glass	≤ 6°C	None	14 days	100 mL
Ammonia	Plastic/Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> to pH<2	28 days	400 mL
BOD 5 Day	Plastic/Glass	≤ 6°C	None	48 hours	1000 mL
Boron	Plastic <sup>5</sup>	None	HNO <sub>3</sub> to pH<2	6 months	200 mL
Bromide	Plastic/Glass	None	None	28 days	100 mL
CBOD 5 Day	Plastic/Glass	≤ 6°C	None	48 hours	1000 mL
COD	Plastic/Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> to pH<2	28 days	100 mL
Chloride	Plastic/Glass	None	None	28 days	50 mL
Chlorine, Residual	Plastic/Glass	None	None	15 min. <sup>6</sup>	200 mL
Color	Plastic/Glass	≤ 6°C	None	48 hours	50 mL
Cyanide –Total <sup>16, 17</sup>	Plastic/Glass	≤ 6°C	NaOH to pH >12, 0.6 g ascorbic Acid <sup>7</sup>	14 days	100 mL
Cyanide – Amenable <sup>16, 17</sup>	Plastic/Glass	≤ 6°C	NaOH to pH >12, 0.6 g ascorbic Acid <sup>7</sup>	14 days	100 mL
Fluoride	Plastic	None	None	28 days	300 mL
Hardness	Plastic/Glass	None	HNO <sub>3</sub> to pH<2 <sup>8</sup>	6 months	100 mL
Hexavalent Chromium	Plastic/Glass	≤ 6°C	Ammonium sulfate buffer pH = 9.3 - 9.7	28 days / 24 hrs <sup>15</sup>	200 mL
Hydrogen Ion (pH)	Plastic/Glass	None	None	15 min. <sup>6</sup>	200 mL
Kjeldahl and organic Nitrogen	Plastic/Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> to pH <2	28 days	500 mL
Mercury <sup>11</sup>	Plastic/Glass	None	HNO <sub>3</sub> to pH<2	28 days	200 mL
Metals <sup>9,10</sup>	Plastic/Glass	None	HNO <sub>3</sub> to pH<2 <sup>18</sup>	6 months	200 mL
Nitrate	Plastic/Glass	≤ 6°C	None	48 hours	100 mL
Nitrate-Nitrite	Plastic/Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> to pH <2	28 days	100 mL
Nitrite	Plastic/Glass	≤ 6°C	None	48 hours	100 mL
Oil and Grease	Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> or HCl to pH <2	28 days	1 L

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION <sup>2,3</sup>		HOLDING TIME <sup>4</sup>	SAMPLE VOLUME
		Temp <sup>14</sup>	Chemical		
Organic Carbon (TOC)	Plastic/Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> or HCl to pH <2 <sup>12</sup>	28 days	250 mL
Orthophosphate	Plastic/Glass	≤ 6°C	Filter within 15 min.	48 hours	250 mL
Oxygen, Dissolved Probe	Glass <sup>13</sup>	None	None	15 min. <sup>6</sup>	200 mL
Oxygen, Winkler	Glass <sup>13</sup>	None	Fix on site and store in dark.	8 hours	300 mL
Phenols	Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> to pH <2	28 days	500 mL
Phosphorus, Elemental	Glass	≤ 6°C	None	48 hours	250 mL
Phosphorus, Total	Plastic/Glass	≤ 6°C	H <sub>2</sub> SO <sub>4</sub> to pH <2	28 days	250 mL
Residue, Total	Plastic/Glass	≤ 6°C	None	7 days	1 L
Residue, Filterable	Plastic/Glass	≤ 6°C	None	7 days	1 L
Residue, Non-Filterable	Plastic/Glass	≤ 6°C	None	7 days	1 L
Residue, Settleable	Plastic/Glass	≤ 6°C	None	48 hours	1 L
Residue, Volatile	Plastic/Glass	≤ 6°C	None	7 days	1 L
Silica	Plastic <sup>5</sup>	≤ 6°C	None	28 days	250 mL
Specific Conductance	Plastic/Glass	≤ 6°C	None	28 days	250 mL
Sulfate	Plastic/Glass	≤ 6°C	None	28 days	250 mL
Sulfide	Plastic/Glass	≤ 6°C	Zinc acetate plus NaOH to pH>9	7 days	500 mL
Sulfite	Plastic/Glass	None	None	15 min. <sup>6</sup>	200 mL
Surfactants	Plastic/Glass	≤ 6°C	None	48 hours	1 L
Temperature	Plastic/Glass	None	None	N/A	100 mL
Turbidity	Plastic/Glass	≤ 6°C	None	48 hours	1 L

**Key to Table**

1. Plastic should be Polyethylene.
2. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at ≤ 6°C until compositing and sample splitting is completed.

**Key to Table**

3. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO<sub>3</sub>) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H<sub>2</sub>SO<sub>4</sub>) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater; and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
4. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
5. May also be collected in quartz or PTFE Plastic.
6. For compliance testing, the analysis must be performed in the field at the time of analysis. If transported to the laboratory for analysis, the analysis will be performed as soon as practical and reported qualified.
7. Should only be used in the presence of residual chlorine. (Alternatively, sodium arsenite may be used.)
8. H<sub>2</sub>SO<sub>4</sub> to a pH <2 is also acceptable.
9. Except Mercury and Hexavalent Chromium.
10. For dissolved metals, samples must be filtered on site before adding HNO<sub>3</sub> preservative (or before shipping to laboratory).
11. Samples collected for determination of trace level mercury (100 ng/L) using EPA 1631 must be collected in tightly capped Fluor polymer or glad bottles and preserved with BrCl or HCl solution within 48 hours of sample collection. The time to preservation may be extended to 28 days if a sample is oxidized in the sample bottle. Samples collected for dissolved trace level mercury should be filtered in the laboratory. However, if circumstances prevent overnight shipping, samples should be filtered in a designated clean area in the field in accordance with procedures given in Method 1669. Samples that been collected for determination of total or dissolved trace level mercury must be analyzed within 90 days of sample collection.
12. Phosphoric acid (H<sub>3</sub>PO<sub>4</sub>) may also be used.
13. Should have glass lid or top.
14. Aqueous samples must be preserved at ≤6 °C unless otherwise indicated, and should not be frozen unless data demonstrating that sample freezing does not adversely impact sample integrity is maintained on file and accepted as valid by the regulatory authority. Also, for purposes of NPDES monitoring, the specification of "≤ °C" is used in place of the "4 °C" and "<4 °C" sample temperature requirements listed in some methods. It is not necessary to measure the sample temperature to three significant figures (1/100th of 1 degree); rather, three significant figures are specified so that rounding down to 6 °C may not be used to meet the ≤6 °C requirement. The preservation temperature does not apply to samples that are analyzed immediately (less than 15 minutes).
15. Holding time is 24 hours if pH adjustment is not performed.
16. In the Field: Samples are to be tested for Sulfide using lead acetate paper prior to the addition of Sodium Hydroxide (NaOH). If sulfide is present, the sample must be treated with Cadmium Chloride and filtered prior to the addition of NaOH. If the sulfide test and treatment is not performed in the field, the lab will test the samples for sulfide using lead acetate paper at the time of receipt and if sulfide is present in the sample, the client will be notified and given the option of retaking the sample and treating in the field per the method requirements or the laboratory can analyze the samples as delivered (with sulfide treatment by laboratory) and qualify the results in the final report.
17. It is the responsibility of the client to notify the laboratory if thiosulfate, sulfite, or thiocyanate are known or suspected to be present in the sample. This notification may be on the chain of custody. The samples may need to be subcontracted to a laboratory that performs a UV digestion. If the lab does not perform the UV digestion on samples that contain these compounds, the results must be qualified in the final report.
18. Acid preservation may be omitted for shipping and laboratory will acidify at least 24 hours prior to analysis.

**Table 23-4  
Holding Times, Preservation and Container Requirements: NPDES - Organic**

PARAMETER	CONTAINER	PRESERVATION <sup>1,2</sup>		HOLDING TIME <sup>3</sup>	SAMPLE VOLUME
		Temp. <sup>15</sup>	Chemical		
Purgeable Halocarbons	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5</sup>	14 days	40 mL
Purgeable Aromatic Hydrocarbons	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5</sup> , HCl to pH<2	14 days <sup>6</sup>	40 mL
Acrolein and Acrylonitrile	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5</sup> , adjust pH to 4-5 <sup>7</sup>	14 days	40 mL
Phenols <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5</sup>	7 days <sup>8</sup>	1 L
Benzidines <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5</sup>	7 days <sup>8, 11</sup>	1 L
Phthalate esters <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	None	7 days <sup>8</sup>	1 L
Nitrosamines <sup>9,12</sup>	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5,13</sup>	7 days <sup>8</sup>	1 L
PCBs <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	None	1 year <sup>8</sup>	1 L
Nitroaromatics and Isophorone <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5,13</sup>	7 days <sup>8</sup>	1 L
Polynuclear Aromatic Hydrocarbons <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5,13</sup>	7 days <sup>8</sup>	1 L
Haloethers <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5</sup>	7 days <sup>8</sup>	1 L
Chlorinated Hydrocarbons <sup>9</sup>	Glass <sup>4</sup>	≤ 6°C	None	7 days <sup>8</sup>	1 L
CDD/CDFs <sup>9</sup> – Aqueous: Field/Lab Preservation	Glass	≤ 6°C	pH <9, 0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>5</sup>	1 year	1 L
CDD/CDFs <sup>9</sup> – Solids/Mixed Phase/ - Field Preservation	Glass	≤ 6°C	None	7 days	1 L
CDD/CDFs <sup>9</sup> – Tissue – Field Preservation	Glass	≤ 6°C	None	24 hours	
CDD/CDFs <sup>9</sup> – Solids/Mixed Phase/Tissue - Lab Preservation	Glass	< -10°C	None	1 year	1 L
Pesticides <sup>9</sup>	Glass	≤ 6°C	pH 5-9 <sup>14</sup>	7 days <sup>8</sup>	1 L

### **Key to Table**

1. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at  $\leq 6^{\circ}\text{C}$  until compositing and sample splitting is completed.
2. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid ( $\text{HNO}_3$ ) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid ( $\text{H}_2\text{SO}_4$ ) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
3. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
4. With Teflon lined septum.
5. Should only be used in the presence of residual chlorine. Ascorbic may be used instead.
6. Samples receiving no pH adjustments must be analyzed within 7 days. If 2-chlorovinylethylether is a target analyte, the sample should not be acidified.
7. The pH adjustment is not required if acrolein is not being measured. Samples for acrolein receiving no pH adjustment must be analyzed within three days of sampling.
8. 7 days until extraction, 40 days after extraction. (PCB only – 1 year after extraction)
9. When the extractable analytes of concern fall within a single chemical category, the specified preservative and maximum holding times should be observed for optimum safeguard of sample integrity. When the analytes of concern fall within two or more categories, the sample may be preserved by cooling to  $\leq 6^{\circ}\text{C}$  reducing residual chlorine with 0.0008 % sodium thiosulfate, storing in the dark, and adjusting the pH to 6-9. Samples preserved in this manner may be held for 7 days before extraction and for 40 days after extraction. Exceptions to this optional preservation and holding time procedure are noted in footnote 5 (re the requirement for thiosulfate reduction of residual chlorine) and footnotes 10 and 11(re the analysis of Benzidine).
10. If 1,2-diphenylhydrazine is likely to be present, adjust pH to of the sample to  $4.0 \pm 0.2$  to prevent rearrangement to benzidine.
11. Extracts may be stored up to 30 days before analysis if storage temperature is  $< 0^{\circ}\text{C}$ .
12. For the analysis of diphenylnitrosamine, add 0.008 %  $\text{Na}_2\text{S}_2\text{O}_3$  and adjust pH to 7-10 with NaOH within 24 hours of sampling.
13. Store in dark.
14. The pH adjustment may be performed upon receipt in the laboratory and may be omitted if the samples are extracted within 72 hours of collection. For the analysis of aldrin, add 0.0008 %  $\text{Na}_2\text{S}_2\text{O}_3$ .
15. Aqueous samples must be preserved at  $\leq 6^{\circ}\text{C}$  unless otherwise indicated, and should not be frozen unless data demonstrating that sample freezing does not adversely impact sample integrity is maintained on file and accepted as valid by the regulatory authority. Also, for purposes of NPDES monitoring, the specification of " $\leq^{\circ}\text{C}$ " is used in place of the " $4^{\circ}\text{C}$ " and " $<4^{\circ}\text{C}$ " sample temperature requirements listed in some methods. It is not necessary to measure the sample temperature to three significant figures (1/100th of 1 degree); rather, three significant figures are specified so that rounding down to  $6^{\circ}\text{C}$  may not be used to meet the  $\leq 6^{\circ}\text{C}$  requirement. The preservation temperature does not apply to samples that are analyzed immediately (less than 15 minutes).

**Table 23-5.  
 Holding Times, Preservation and Container Requirements: NPDES - Radiological**

PARAMETER	CONTAINER	PRESERVATION <sup>1,2</sup>		HOLDING TIME <sup>3</sup>	SAMPLE VOLUME
		Temp.	Chemical		
Alpha, Beta, Radium	Plastic/Glass	None	HNO <sub>3</sub> to pH<2	6 months	1 L

**Key to Table**

1. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
2. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Nitric acid (HNO<sub>3</sub>) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater).
3. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.

**Table 23-6.**  
**Holding Times, Preservation and Container Requirements: RCRA - Aqueous**

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION <sup>2,3</sup>		HOLDING TIME <sup>4</sup>	SAMPLE VOLUME
		Temp. <sup>12</sup>	Chemical		
Chloride	Plastic/Glass	4°C	None	28 days	100 mL
Cyanide -Total	Plastic/Glass	4°C	NaOH to pH >12 <sup>5</sup>	14 days	250 mL
Cyanide -Amenable	Plastic/Glass	4°C	NaOH to pH >12 <sup>5</sup>	14 days	250 mL
Hydrogen Ion (pH)	Plastic/Glass	4°C	None	24 hours <sup>11</sup>	100 mL
Nitrate	Plastic/Glass	4°C	None	48 hours	28 days
Oil and Grease	Glass	4°C	HCl	28 days	1 L
Organic carbon (TOC)	Plastic/Glass	4°C	pH to <2 <sup>6</sup> Store in dark	28 days	28 days
Sulfate	Plastic/Glass	4°C	None	28 days	400 mL
Sulfide	Plastic/Glass	4°C	Add Zn Acetate	7 days	400 mL
Chromium VI	Plastic/Glass	4°C	None	24 hours	250 mL
Mercury	Plastic/Glass	None	HNO <sub>3</sub> to pH<2	28 days	250 mL
Other Metals	Plastic/Glass	None	HNO <sub>3</sub> to pH<2	6 months	250 mL
Acrolein and Acrylonitrile	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup> Adjust pH to 4-5 <sup>13</sup>	14 days	1 L
Benzidines	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup>	7 days <sup>8</sup>	1 L
Chlorinated Hydrocarbons	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup>	7 days <sup>8</sup>	1 L
Dioxins and Furans	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup>	30 days <sup>8</sup>	1 L
Haloethers	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup>	7 days <sup>8</sup>	1 L
Nitroaromatics and cyclic ketones	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup> , store in dark	7 days <sup>8</sup>	1 L
Nitrosamines	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup> , store in dark	7 days <sup>8</sup>	1 L
Organochlorine Pesticides	Glass <sup>10</sup>	4°C	None	7 days <sup>8</sup>	1 L
Organophosphorus Pesticides	Glass <sup>10</sup>	4°C	Adjust pH <sup>9</sup>	7 days <sup>8</sup>	1 L
PCBs	Glass <sup>10</sup>	4°C	None	7 days <sup>8</sup>	1 L
Phenols	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup>	7 days <sup>8</sup>	1 L

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION <sup>2,3</sup>		HOLDING TIME <sup>4</sup>	SAMPLE VOLUME
		Temp. <sup>12</sup>	Chemical		
Phthalate Esters	Glass <sup>10</sup>	4°C	None	7 days <sup>8</sup>	1 L
Polynuclear Aromatic Hydrocarbons	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup> , store in dark	7 days <sup>8</sup>	1 L
Purgeable Hydrocarbons	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup> Adjust pH <2 <sup>2</sup>	14 days	40 mL
Purgeable Halocarbons	Glass <sup>10</sup>	4°C	0.0008 % Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub> <sup>7</sup>	14 days	40 mL
Total Organic Halides (TOX)	Glass <sup>10</sup>	4°C	Adjust pH to <2 with H <sub>2</sub> SO <sub>4</sub>	28 days	1 L
Radiological Tests (Alpha, Beta, Radium)	Plastic/Glass	None	HNO <sub>3</sub> to pH<2	6 months	250 mL

**Key to Table**

1. Plastic should be Polyethylene.
2. Sample preservation should be performed immediately upon sample collection. For composite chemical samples, each aliquot should be preserved at the time of collection. When use of an automated sampler makes it impossible to preserve each aliquot, then chemical samples may be preserved by maintaining at 4°C until compositing and sample splitting is completed.
3. When any sample is to be shipped by common carrier or sent through the United States mails, it must comply with the Department of Transportation Hazardous Materials Regulations (49 CFR Part 172). The person offering such material for transportation is responsible for ensuring compliance. For the preservation requirements of Table 6-8, the Office of Hazardous Materials, Materials Transportation Bureau, Department of Transportation has determined that the Hazardous Materials Regulations do not apply to the following materials: Hydrochloric acid, (HCl) in water, solutions at concentrations of 0.04% by weight or less (pH about 1.96 or greater); Nitric acid (HNO<sub>3</sub>) in water solutions at concentrations of 0.15% by weight or less (pH about 1.62 or greater); Sulfuric acid (H<sub>2</sub>SO<sub>4</sub>) in water solutions at concentrations of 0.35% by weight or less pH about 1.15 or greater); and Sodium hydroxide (NaOH) in water solutions at concentrations of 0.080% by weight or less (pH about 12.30 or less).
4. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
5. If oxidizing agents are present, add 5 mL 0.1 N NaAsO<sub>2</sub> or 0.06 g of ascorbic acid per L. See Cyanide SOP for additional information about other interferences.
6. Adjust pH to <2 with H<sub>2</sub>SO<sub>4</sub>, HCl, or solid NaHSO<sub>4</sub>. Free Chlorine must be removed prior to adjustment.
7. Free Chlorine must be removed by the appropriate addition of Na<sub>2</sub>S<sub>2</sub>O<sub>3</sub>.
8. 7 days until extraction. 40 days after extraction.
9. Adjust pH to 5-8 using NaOH or H<sub>2</sub>SO<sub>4</sub>.
10. With Teflon lined septum.
11. Holding Time is listed as "As Soon as Possible" in SW 846. Per EPA MICE, the recommended maximum holding time for pH in water is 24 hours and pH in soil is 7 days. There are no mandated regulatory requirements.
12. For samples with a temperature requirement of 4°C, a sample temperature of just above the water freezing temperature to ≤ 6°C is acceptable.
13. Based on guidance from EPA MICE, if samples are received without pH adjustment, the holding time is 7 days.

**Table 23-7.  
Holding Times, Preservation and Container Requirements: RCRA – Non-Aqueous**

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION		HOLDING TIME <sup>2</sup>	SAMPLE WEIGHT
		Temp. <sup>7</sup>	Chemical		
Chloride	Glass	4°C	None	28 days	50 g
Cyanide -Total	Glass	4°C	None	14 days	50 g
Cyanide - Amenable	Glass	4°C	None	14 days	50 g
Hydrogen Ion (pH)	Glass	4°C	None	7 days <sup>6</sup>	50 g
Nitrate	Glass	4°C	None	N/A	50 g
Oil and Grease	Glass	4°C	None	28 days	50 g
Sulfide	Glass	4°C	Add Zn Acetate, zero headspace	7 days	50 g
Chromium VI	Glass	4°C	None	30 days	50 g
Mercury	Plastic/Glass	None	None	28 days	50 g
Other Metals	Plastic/Glass	None	None	6 months	50 g
Acrolein and Acrylonitrile	Glass <sup>4</sup>	4°C	None	14 days	50 g
Benzidines	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Chlorinated Hydrocarbons	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Dioxins and Furans	Glass <sup>4</sup>	4°C	None	30 days <sup>3</sup>	50 g
Haloethers	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Nitroaromatics and cyclic ketones	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Nitrosamines	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Organochlorine Pesticides	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Organophosphorus Pesticides	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
PCBs	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Phenols	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Phthalate Esters	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g
Polynuclear Aromatic Hydrocarbons	Glass <sup>4</sup>	4°C	None	14 days <sup>3</sup>	50 g

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION		HOLDING TIME <sup>2</sup>	SAMPLE WEIGHT
		Temp. <sup>7</sup>	Chemical		
Purgeable Hydrocarbons	Glass <sup>4</sup>	4°C	None	14 days <sup>5</sup>	50 g
Purgeable Halocarbons	Glass <sup>4</sup>	4°C	None	14 days <sup>5</sup>	50 g
Total Organic Halides (TOX)	Glass <sup>4</sup>	4°C	None	28 days	50 g

**Key to Table**

1. Plastic should be Polyethylene.
2. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
3. 14 days until extraction. 40 days after extraction.
4. With Teflon Lined Septum.
5. See Volatile SOP for more detailed preservation requirements.
6. Holding Time is listed as "As Soon as Possible" in SW 846. Per EPA MICE, the recommended maximum holding time for pH in water is 24 hours and pH in soil is 7 days. There are no mandated regulatory requirements.
7. For samples with a temperature requirement of 4°C, a sample temperature of just above the water freezing temperature to ≤ 6°C is acceptable.

**Table 23-8.  
 Holding Times, Preservation and Container Requirements: Air Samples**

PARAMETER	CONTAINER <sup>1</sup>	PRESERVATION		HOLDING TIME <sup>2</sup>	SAMPLE WEIGHT
		Temp.	Chemical		
Volatile Organics	Summa Canister	None	None	30 days	6L or 1L
Volatile Organics	Tedlar Bag	None	None	72 hrs <sup>3,4</sup>	1 L

**Key to Table**

1. Plastic should be Polyethylene.
2. Samples should be analyzed as soon as possible after collection. The times listed are the maximum times that samples may be held before analysis and still be considered valid.
3. Holding Time is based on SW 846 Method 0040 "SAMPLING OF PRINCIPAL ORGANIC HAZARDOUS CONSTITUENTS FROM COMBUSTION SOURCES USING TEDLAR® BAGS". Some states specifically enforce this holding time (e.g. Florida, New Jersey) and others have not specified this information in their regulatory requirements.
4. The holding time is 72 hours unless the laboratory has a documented validation study that indicates a longer HT is acceptable for the analytes of interest.

## SECTION 24

### HANDLING OF SAMPLES (NELAC 5.5.8)

Sample management procedures at TestAmerica West Sacramento ensure that sample integrity and custody are maintained and documented from sampling/receipt through disposal.

#### **24.1**      **CHAIN OF CUSTODY (COC)**

The COC form is the written documented history of any sample and can be initiated when bottles are sent to the field, or at the time of sampling. This form is completed by the sampling personnel and accompanies the samples to the laboratory where it is received and stored under the laboratory's custody. The purpose of the COC form is to provide a legal written record of the handling of samples from the time of collection until they are received at the laboratory. It also serves as the primary written request for analyses from the client to the laboratory. The COC form acts as a purchase order for analytical services when no other contractual agreement is in effect. An example of a COC form may be found in Figure 24-1.

##### **24.1.1**      **Field Documentation**

The information the sampler needs to provide at the time of sampling on the container label is:

- Sample identification
- Date and time
- Preservative

During the sampling process, the COC form is completed and must be legible (see Figure 24-1). This form includes information such as:

- Client name, address, phone number and fax number (if available)
- Project name and/or number
- The sample identification
- Date, time and location of sampling
- Sample collectors name
- The matrix description
- The container description
- The total number of each type of container
- Preservatives used
- Analysis requested
- Requested turnaround time (TAT)
- Any special instructions
- Purchase Order number or billing information (e.g. quote number) if available
- The date and time that each person received or relinquished the sample(s), including their signed name.

The samples are stored in a cooler with ice, as applicable, and remain solely in the possession of the client's field technician until the samples are delivered to the laboratory. The sample collector must assure that each container is in his/her physical possession or in his/her view at all times, or stored in such a place and manner to preclude tampering. The field technician relinquishes the samples in writing on the COC form to the sample control personnel at the laboratory or to a TestAmerica courier. Samples are only considered to be received by lab when personnel at the laboratory have physical contact with the samples.

**Note:** Independent couriers are not required to sign the COC form. The COC is usually kept in the sealed sample cooler. The receipt from the courier is stored with the COC.

#### **24.1.2 Legal / Evidentiary Chain-of-Custody**

If samples are identified for legal/evidentiary purposes on the COC, legal COCs will be generated per the Manual for Certification of Laboratories Analyzing Drinking Water, Fifth Edition, January 2005, Appendix A, and SOP No. WS-QA-0003, "Sample Receipt and Procedures".

#### **24.2 SAMPLE RECEIPT**

Samples are received at the laboratory by designated sample receiving personnel and a unique laboratory project identification number is assigned. Each sample container shall be assigned a unique sample identification number that is cross-referenced to the client identification number such that traceability of test samples is unambiguous and documented. Each sample container is affixed with a durable sample identification label. Sample acceptance, receipt, tracking and storage procedures are summarized SOP No. WS-QA-0003, "Sample Receipt and Procedures".

##### **24.2.1 Sample Log-in**

Refer to SOP No. SAC-QA-003, "Sample Receipt Procedures" for details of sample log-in requirements.

Each job/set of samples is logged into LIMS with a minimum of the following information:

- Client Name, Project Name, Address, Phone, Fax, Report to information, invoice to information (most of this information is "default information" that is stored in the LIMS)
- Date and time sampled
- Date and time received
- Job and/or project description, sample description
- Sample matrix, special sample remarks
- Reporting requirements (i.e., QC level, report format, invoicing format);
- Turn-around-time requirements
- Parameters (methods and reporting limits or MDLs are default information for a given parameter).

### **24.3 SAMPLE ACCEPTANCE POLICY**

The laboratory has a written sample acceptance policy (Figure 24-2) that clearly outlines the circumstances under which samples shall be accepted or rejected. These include:

- A COC filled out completely
- Samples must be properly labeled
- Proper sample containers with adequate volume for the analysis and necessary QC
- Samples must be preserved according to the requirements of the requested analytical method
- Sample holding times must be adhered to
- All samples submitted for water/solid Volatile Organic analyses must have a Trip Blank submitted at the same time
- All samples submitted for chemical warfare degradate analysis must be screened for the presence of agent prior to shipment
- The project manager will be notified if any sample is received in damaged condition.

Data from samples which do not meet these criteria are flagged and the nature of the variation from policy is defined. A copy of the sample acceptance policy is provided to each client prior to shipment of samples.

### **24.4 SAMPLE STORAGE**

In order to avoid deterioration, contamination or damage to a sample during storage and handling, from the time of receipt until all analyses are complete, samples are stored in refrigerators suitable for the sample matrix. In addition, samples to be analyzed for volatile organic parameters are stored in separate refrigerators designated for volatile organic parameters only. Samples are never to be stored with reagents, standards or materials that may create contamination.

To ensure the integrity of the samples during storage, refrigerator blanks are maintained in the volatile sample refrigerators and analyzed every two weeks.

Analysts and technicians retrieve the sample container allocated to their analysis from the designated refrigerator and place them on carts, analyze the sample, and return the remaining sample or empty container to the refrigerator from which it originally came. All unused portions of samples, including empty sample containers, are returned to the secure sample control area. All samples are kept in the refrigerators for 30 days past invoicing, unless other arrangements have been made with the client.

Access to the laboratory is controlled such that sample storage need not be locked at all times unless a project specifically demands it. Samples are accessible to laboratory personnel only. Visitors to the laboratory are prohibited from entering the refrigerator and laboratory areas unless accompanied by an employee of TestAmerica.

### **24.5 HAZARDOUS SAMPLES AND FOREIGN SOILS**

Foreign soil samples are sent out for incineration by a USDA-approved waste disposal facility.

#### **24.6 SAMPLE SHIPPING**

In the event that the laboratory needs to ship samples, the samples are placed in a cooler with enough ice to ensure the samples remain just above freezing and at or below 6.0°C during transit. The samples are carefully surrounded by packing material to avoid breakage (yet maintain appropriate temperature). For sample shipments which include water/solid volatile organic analyses, a trip blank is enclosed when required by method specifications or state or regulatory programs. The chain-of-custody form is signed by the sample control technician and attached to the shipping paperwork. Samples are generally shipped overnight express or hand-delivered by a TestAmerica courier to maintain sample integrity. All personnel involved with shipping and receiving samples must be trained to maintain the proper chain-of-custody documentation and to keep the samples intact and on ice. The Environmental, Health and Safety Manual contains additional shipping requirements.

#### **24.7 SAMPLE DISPOSAL**

Samples should be retained for a minimum of 30 days after the project report is sent, however, provisions may be made for earlier disposal of samples once the holding time is exceeded. Some samples are required to be held for longer periods based on regulatory or client requirements (e.g., 60 days after project report is sent). The laboratory must follow the longer sample retention requirements where required by regulation or client agreement. Several possibilities for sample disposal exist: the sample may be consumed completely during analysis, the sample may be returned to the customer or location of sampling for disposal, or the sample may be disposed of in accordance with the laboratory's waste disposal procedures (SOP: SAC-EHS-001, "Waste Disposal"). All procedures in the laboratory Environmental, Health and Safety Manual are followed during disposal. Samples are normally maintained in the laboratory no longer than one month from receipt unless otherwise requested. Unused portions of samples found or suspected to be hazardous according to state or federal guidelines may be returned to the client upon completion of the analytical work.



**Figure 24-2.**

**Sample Acceptance Policy**

NELAC and TestAmerica West Sacramento have specific requirements under which all samples will be received by the laboratory for analysis. TestAmerica West Sacramento will review your sample shipment against those requirements as listed below, and will communicate any discrepancies to you. Your project manager will assist you in the appropriate resolution of any issues related to sample receipt. Please contact your project manager with any questions.

TestAmerica West Sacramento requirements are as follows:

- ✓ Proper, full and complete documentation, which includes sample identification, the location, date and time of collection, the collector's name, the preservation type, the sample matrix type, the requested testing method, and any special remarks concerning the samples, shall be provided.
- ✓ Samples must be accompanied by written disclosure of the known or suspected presence of any hazardous substances, as defined by applicable federal or state law.
- ✓ Each sample shall be collected in the appropriate sample container and labeled with unique, durable and indelible identification.
- ✓ Drinking waters samples for Method 1613B that may have residual chlorine must be checked and treated in the field, or collected in sodium thiosulfate preserved containers.
- ✓ The samples shall arrive at the laboratory with adequate remaining holding time for the analyses requested.
- ✓ Sufficient sample volume must be available to perform the requested analyses.
- ✓ Received samples must not exhibit obvious signs of damage, contamination or inadequate preservation.
- ✓ For samples undergoing chemical warfare degradate analysis, the sample must be screened for agent prior to shipment in accordance with appendix 10 of our Sample Receipt Procedure (WS-QA-0003).
- ✓ Samples containing mammalian tissue will not be accepted without prior coordination with a project manager. Additional conditions for receipt and handling of tissue are outlined in Appendix 11 of our Sample Receipt Procedure (WS-QA-0003).

The laboratory will notify the client/Project Manager upon sample receipt if the samples fail to meet any of the above requirements.

When completing the chain of custody form, please do not forget to sign your name in the "relinquished by" box.

## SECTION 25.0

### ASSURING THE QUALITY OF TEST RESULTS (NELAC 5.5.9)

#### 25.1 OVERVIEW

In order to assure our clients of the validity of their data, the laboratory continuously evaluates the quality of the analytical process. The analytical process is controlled not only by instrument calibration as discussed in Section 21, but also by routine process quality control measurements (e.g. Blanks, Laboratory Control Samples (LCS), Matrix Spikes (MS), duplicates (DUP), surrogates, Internal Standards (IS)). These quality control checks are performed as required by the method or regulations to assess precision and accuracy. In addition to the routine process quality control samples, Proficiency Testing (PT) Samples (concentrations unknown to laboratory) are analyzed to help ensure laboratory performance.

#### 25.2 CONTROLS

Sample preparation or pre-treatment is commonly required before analysis. Typical preparation steps include homogenization, grinding, solvent extraction, sonication, acid digestion, distillation, reflux, evaporation, drying and ashing. During these pre-treatment steps, samples are arranged into discreet manageable groups referred to as preparation (prep) batches. Prep batches provide a means to control variability in sample treatment. Control samples are added to each prep batch to monitor method performance and are processed through the entire analytical procedure with investigative/field samples.

#### 25.3 NEGATIVE CONTROLS

**25.3.1 Method Blanks** are used to assess preparation and analysis for possible contamination during the preparation and processing steps.

**25.3.1.1** The method blank is prepared from a clean matrix similar to that of the associated samples that is free from target analytes (e.g., Reagent water, Ottawa sand, glass beads, etc.) and is processed along with and under the same conditions as the associated samples.

**25.3.1.2** The method blank goes through all of the steps of the process (including as necessary: filtration, clean-ups, etc.).

**25.3.1.3** The specific frequency of use for method blanks during the analytical sequence is defined in the specific standard operating procedure for each analysis. Generally it is 1 for each batch of samples; not to exceed 20 environmental samples.

**25.3.1.4** Evaluation criteria and corrective action for method blanks is defined in the specific standard operating procedure for each analysis. Generally, corrective action is taken if the concentration of a target analyte in the blank is at or above the reporting limit as established by the method or regulation.

- The source of contamination is investigated

- Measures are taken to minimize or eliminate the source of the contamination
- Affected samples are reprocessed or the results are qualified on the final report.

**25.3.2** **Calibration Blanks** are prepared and analyzed along with calibration standards where applicable. They are prepared using the same reagents that are used to prepare the standards. In some analyses the calibration blank may be included in the calibration curve.

**25.3.3** **Instrument Blanks** are blank reagents or reagent water that may be processed during an analytical sequence in order to assess contamination in the analytical system. In general, instrument blanks are used to differentiate between contamination caused by the analytical system and that caused by the sample handling or sample prep process. Instrument blanks may also be inserted throughout the analytical sequence to minimize the effect of carryover from samples with high analyte content.

**25.3.4** **Trip Blanks** are required to be submitted by the client with each shipment of samples requiring aqueous and solid volatiles analyses. Additionally, trip blanks may be prepared and analyzed for volatile analysis of air samples, when required by the client. A trip blank may be purchased (certified clean) or is prepared by the laboratory by filling a clean container with pure deionized water that has been purged to remove any volatile compounds. Appropriate preservatives are also added to the container. The trip blank is sent with the bottle order and is intended to reflect the environment that the containers are subjected to throughout shipping and handling and help identify possible sources if contamination is found. The field sampler returns the trip blank in the cooler with the field samples. Trip Blanks are also sometimes referred to as Travel Blanks.

**25.3.5** **Field Blanks** are sometimes used for specific projects by the field samplers. A field blank is prepared in the field by filling a clean container with pure reagent water and appropriate preservative, if any, for the specific sampling activity being undertaken. (EPA OSWER)

**25.3.6** **Equipment Blanks** are also sometimes created in the field for specific projects. An equipment blank is a sample of analyte-free media which has been used to rinse common sampling equipment to check effectiveness of decontamination procedures. (NELAC)

**25.3.7** **Holding Blanks**, also referred to as refrigerator or freezer blanks, are used to monitor the sample storage units for volatile organic compounds during the storage of VOA samples in the laboratory (refer to Section 24.4).

**25.3.8** **Field blanks**, equipment blank and trip blanks, when received, are analyzed in the same manner as other field samples. When known, blanks should not be selected for matrix QC, as it does not provide information on the behavior of the target compounds in the field samples. Usually, the client sample ID will provide information to identify the field blanks with labels such as "FB", "EB", or "TB".

## **25.4** **POSITIVE CONTROLS**

Control samples (e.g., QC indicators) are analyzed with each batch of samples to evaluate data based upon (1) Method Performance (Laboratory Control Sample (LCS) or Blank Spike (BS)), which entails both the preparation and measurement steps; and (2) Matrix Effects (Matrix Spike

(MS) (Matrix spikes are not applicable to air) or Sample Duplicate (MD, DUP), which evaluates field sampling accuracy, precision, representativeness, interferences, and the effect of the matrix on the method performed. Each regulatory program and each method within those programs specify the control samples that are prepared and/or analyzed with a specific batch

Note that frequency of control samples vary with specific regulatory, methodology and project specific criteria. Complete details on method control samples are as listed in each analytical SOP.

#### **25.4.1 Method Performance Control - Laboratory Control Sample (LCS)**

**25.4.1.1** The LCS measures the accuracy of the method in a blank matrix and assesses method performance independent of potential field sample matrix affects in a laboratory batch.

**25.4.1.2** The LCS is prepared from a clean matrix similar to that of the associated samples that is free from target analytes (for example: Reagent water, Ottawa sand, glass beads, etc.) and is processed along with and under the same conditions as the associated samples. The LCS is spiked with verified known amounts of analytes or is made of a material containing known and verified amounts of analytes, taken through all preparation and analysis steps along with the field samples. Where there is no preparation taken for an analysis (such as in aqueous volatiles), or when all samples and standards undergo the same preparation and analysis process (such as Phosphorus), a calibration verification standard is reported as the LCS. In some instances where there is no practical clean solid matrix available, aqueous LCSs may be processed for solid matrices; final results may be calculated as mg/kg or ug/kg, assuming 100% solids and a weight equivalent to the aliquot used for the corresponding field samples, to facilitate comparison with the field samples.

**25.4.1.3** Certified pre-made reference material purchased from a NIST/A2LA accredited vendor may also be used for the LCS when the material represents the sample matrix or the analyte is not easily spiked (e.g. solid matrix LCS for metals, TDS, etc.).

**25.4.1.4** As stated in the opening of this section, the LCS goes through all of the steps of the process (including as necessary: filtration, clean-ups, etc.).

**25.4.1.5** The specific frequency of use for LCS during the analytical sequence is defined in the specific standard operating procedure for each analysis. It is generally 1 for each batch of samples; not to exceed 20 environmental samples.

**25.4.1.6** If the mandated or requested test method, or project requirements, do not specify the spiking components, the laboratory shall spike all reportable components to be reported in the Laboratory Control Sample (and Matrix Spike) where applicable (e.g. no spike of pH). However, in cases where the components interfere with accurate assessment (such as simultaneously spiking chlordane, toxaphene and PCBs in Method 608), the test method has an extremely long list of components or components are incompatible, at a minimum, a representative number of the listed components (see below) shall be used to control the test method. The selected components of each spiking mix shall represent all chemistries, elution patterns and masses, permit specified analytes and other client requested components. However,

the laboratory shall ensure that all reported components are used in the spike mixture within a two-year time period.

**25.4.1.6.1** For methods that have 1-10 target analytes, spike all components.

**25.4.1.6.2** For methods that include 11-20 target analytes, spike at least 10 or 80%, whichever is greater.

**25.4.1.6.3** For methods with more than 20 target analytes, spike at least 16 components.

**25.4.1.6.4** Exception: Due to analyte incompatibility in pesticides, Technical Chlordane is only spiked at client request based on specific project needs.

**25.4.1.6.5** Exception: Due to analyte incompatibility between the various PCB aroclors, aroclors 1016 and 1260 are used for spiking as they cover the range of all of the aroclors. Specific aroclors may be used by request on a project specific basis.

**25.4.1.7** **Accuracy Calculation**: Percent Recovery (%R) Calculation (applies to LCS, CCV, Surrogates, and Matrix Spikes).

$$\%R = \frac{AV}{TV} \times 100$$

Where: AV = Analyzed Value  
TV = True Value

## **25.5** **SAMPLE MATRIX CONTROLS**

### **25.5.1** **Matrix Spikes (MS)**

**25.5.1.1** The Matrix spike is used to assess the effect sample matrix of the spiked sample has on the precision and accuracy of the results generated by the method used.

**25.5.1.2** An MS is essentially a sample fortified with a known amount of the test analyte(s). At a minimum, with each matrix-specific batch of samples processed, an MS is carried through the complete analytical procedure. Unless specified by the client, samples used for spiking are randomly selected and rotated between different client projects.

**25.5.1.3** If the mandated or requested test method does not specify the spiking components, the laboratory shall spike all reportable components to be reported in the Laboratory Control Sample and Matrix Spike. However, in cases where the components interfere with accurate assessment (such as simultaneously spiking chlordane, toxaphene and PCBs in Method 608), the test method has an extremely long list of components or components are incompatible, a representative number of the listed components (see LCS analytes 25.4.1.6 above) may be used to control the test method. The selected components of each spiking mix shall represent all chemistries, elution patterns and masses, permit-specified analytes and other client requested components. However, the laboratory shall ensure that all reported components are used in the spike mixture within a two-year time period.

**25.5.1.4** The percent recovery calculation for matrix spikes is essentially the same as the calculation shown in 25.4.1.7 except that:

$$AV = Sp - Sa$$

Where: Sp = Spike result  
Sa = Sample result

### **25.5.2** Surrogate Spikes

**25.5.2.1** Surrogate Spikes are similar to matrix spikes except the analytes are compounds with properties that mimic the analyte of interest and are unlikely to be found in environmental samples.

**25.5.2.2** Surrogate compounds are added to all samples, standards, and blanks, for all organic chromatography methods except when the matrix precludes its use or when a surrogate is not available. The recovery of the surrogates is compared to the acceptance limits for the specific method (also refer to Section 25.5). Poor surrogate recovery may indicate a problem with sample composition and shall be reported, with data qualifiers, to the client whose sample produced poor recovery.

### **25.5.3** Duplicates

**25.5.3.1** For a measure of analytical precision, with each matrix-specific batch of samples processed, a matrix duplicate (MD or DUP) sample, matrix spike duplicate (MSD), or LCS duplicate (LCSD) is carried through the complete analytical procedure. Duplicate samples are usually analyzed with methods that do not require matrix spike analysis. LCSDs are normally not performed except when regulatory agencies or client specifications require them. The recoveries for the spiked duplicate samples must meet the same laboratory established recovery limits as the accuracy QC samples. If an LCSD is analyzed both the LCS and LCSD must meet the same recovery criteria and be included in the final report. The precision measurement is reported as "Relative Percent Difference" (RPD). Poor precision between duplicates (except LCS/LCSD) may indicate non-homogeneous matrix or sampling.

#### **25.5.3.2** Precision Calculation (Relative Percent Difference - RPD)

$$RPD = \frac{|S - D|}{\frac{(S + D)}{2}} \times 100$$

Where: S=Sample Concentration  
D=Duplicate Concentration

### **25.5.4** Internal Standards

**25.5.4.1** In most organic analyses, internal standards are spiked into all environmental and quality control samples (including the initial calibration standards). An internal

standard is also used with some metals analyses. It is added to sample extracts after the extraction (post-prep). The acceptance criteria in most methods are 50% to 200% of the responses in the mid-point of the corresponding calibration curve. Consult the method-specific SOPs for details on the internal standard compounds, calculations and acceptance criteria.

**25.5.4.2** When the internal standard recoveries fall outside these limits, if there are not obvious chromatographic interferences, reanalyze the sample to confirm a possible matrix effect. If the recoveries confirm or there was obvious interference, results are reported from the original analysis and a qualifier is added. If the reanalysis meets internal standard recovery criteria, the second run is reported (or both are reported if requested by the client).

## **25.6**      **ACCEPTANCE CRITERIA (CONTROL LIMITS)**

**25.6.1** Each individual analyte in the LCS, MS, or Surrogate Spike are evaluated against the control limits as published in the test method. Where there are no established acceptance criteria, the laboratory calculates control limits with the use of control charts or, in some cases, utilizes client project specific or regulatory mandated control limits. When this occurs, the regulatory or project limits will supersede the laboratory's in-house limits.

**Note:** For methods, analytes and matrices with very limited data (e.g., unusual matrices not analyzed often), interim limits are established using available data or by analogy to similar methods or matrices.

**25.6.2** Once control limits have been established, they are verified, reviewed, and updated if necessary on an annual basis unless the method requires more frequent updating (e.g. EPA SW846 8000 series methods). Control limits are established per method (as opposed to per instrument) regardless of the number of instruments utilized.

**25.6.2.1** The lab should consider the effects of the spiking concentration control limits, and to avoid censoring of data. The acceptance criteria for recovery and precision are often a function of the spike concentration used. Therefore, caution must be used when pooling data to generate control limits.

**25.6.2.2** Not only should the results all be from a similar matrix, but the spiking levels should also be approximately the same (within a factor of 2). Similarly, the matrix spike and surrogate results should all be generated using the same set of extraction, cleanup and analysis techniques. For example, results from solid samples extracted by ultrasonic extraction are not mixed with those extracted by Soxhlet.

**25.6.2.3** The laboratory should try and avoid discarding data that do not meet a preconceived notion of acceptable performance. This results in a censored data set, which, when used to develop acceptance criteria, will lead to unrealistically narrow criteria. For a 99% confidence interval, 1 out of every 100 observations likely will still fall outside the limits. For methods with long analyte lists this may mean occasional failures every batch or two. While professional judgment is important in evaluating data to be used to develop acceptance criteria, specific results are not discarded simply because they do not meet one's expectations. However, data points shall be

discarded if they were the result of human or mechanical error or sample concentration exceeded spike level by > 4x.

**25.6.3** Laboratory generated % Recovery acceptance (control) limits are generally established by taking  $\pm 3$  Standard Deviations (99% confidence level) from the average recovery of a minimum of 20-30 data points (more points are preferred).

**25.6.3.1** Regardless of the calculated limit, the limit should be no tighter than the Calibration Verification (ICV/CCV), unless the analytical method specifies a tighter limit.

**25.6.3.2** In-house limits cannot be any wider than those mandated in a regulated analytical method.

**25.6.3.3** The lowest acceptable recovery limit will be 10% (the analyte must be detectable).

**25.6.4** The lab must be able to generate a current listing of their control limits and track when the updates are performed. In addition, the laboratory must be able to recreate historical control limits. Refer to Policy No. WS-PQA-003, "Quality Control Program" for details of the laboratory's procedure.

**25.6.4.1** Current control limits are available in the LIMS, and summary print-outs may be generated at any time using the QC Browser tool. Unless otherwise required by the reference method or a client QAPP, the limits are generated from laboratory data. When new limits are generated, the old limits are maintained in files in the QA office or archived off-site. A separate database tracks generation and effective dates for each set of control limits, and permits retrieval of superseded limits as required.

**25.6.5** An LCS that is within the acceptance criteria establishes that the analytical system is in control and is used to validate the process. Samples that are analyzed with an LCS with recoveries outside of the acceptance limits may be determined as out of control and should be reanalyzed if possible. If reanalysis is not possible, then the results for all affected analytes for samples within the same batch must be qualified when reported. The internal corrective action process (see Section 13) is also initiated if an LCS exceeds the acceptance limits. Sample results may be qualified and reported without reanalysis if:

**25.6.5.1** The analyte results are below the reporting limit and the LCS is above the upper control limit.

**25.6.5.2** If the analytical results are above the relevant regulatory limit and the LCS is below the lower control limit.

**25.6.5.3** If the analyte is designated as a poor performing analyte. Poor performing analytes are those analytes identified as not performing well with specific methods are labeled "Poor Performers". These compounds generally have low percent recoveries and high standard deviations when the results of LCS are compiled. Specific problems may also be noted by the standard manufacturer. The laboratory maintains a list of these analytes in the SOP No. WS-PQA-003, "Quality Control Program".

**25.6.5.4** Or, for NELAC and Department of Defense (DoD) work, there are an allowable number of Marginal Exceedances (ME):

- <11 analytes – 0 marginal exceedances are allowed
- 11 – 30 Analytes – 1 marginal exceedance is allowed
- 31-50 Analytes – 2 marginal exceedances are allowed
- 51-70 Analytes – 3 marginal exceedances are allowed
- 71-90 Analytes – 4 marginal exceedances are allowed
- > 90 Analytes – 5 marginal exceedances are allowed

**25.6.5.4.1** Marginal exceedances are recovery exceedances between 3 SD and 4 SD from the mean recovery limit (NELAC).

**25.6.5.4.2** Marginal exceedances must be random. If the same analyte exceeds the LCS control limit repeatedly, it is an indication of a systematic problem. The source of the error must be located and corrective action taken. The laboratory has a system to monitor marginal exceedances to ensure that they are random.

**25.6.5.4.3** Though marginal exceedances may be allowed, the data must still be qualified to indicate it is outside of the normal limits.

**25.6.6** If the MS/MSDs do not meet acceptance limits, the MS/MSD and the associated spiked sample is reported with a qualifier for those analytes that do not meet limits. If obvious preparation errors are suspected, or if requested by the client, unacceptable MS/MSDs are reprocessed and reanalyzed to prove matrix interference. A more detailed discussion of acceptance criteria and corrective action can be found in Appendix 4 and in Section 13.

**25.6.7** If a surrogate standard falls outside the acceptance limits, if there is not obvious chromatographic matrix interference, reanalyze the sample to confirm a possible matrix effect. If the recoveries confirm or there was obvious chromatographic interference, results are reported from the original analysis and a qualifier is added. If the reanalysis meets surrogate recovery criteria, the second run is reported (or both are reported if requested by the client). Under certain circumstances with client approval, where all of the samples are from the same location and share similar chromatography, the reanalysis may be performed on a single sample rather than all of the samples and if the surrogate meets the recovery criteria in the reanalysis, all of the affected samples would require reanalysis.

## **25.7**      **METHOD DETECTION LIMITS (MDLs)**

MDLs, calculated as described in Section 20.7, are updated or verified annually, or more often if required by the method.

## **25.8**      **ADDITIONAL PROCEDURES TO ASSURE QUALITY CONTROL**

**25.8.1** The laboratory has written procedures to assure the accuracy of the test method including calibration (see Section 21), use of certified reference materials (see Section 22) and use of PT samples (see Section 16).

**25.8.2** A discussion regarding MDLs, Limit of Detection (LOD) and Limit of Quantitation (LOQ) can be found in Section 20.

**25.8.3** Use of formulae to reduce data is discussed in the method standard operating procedures and in Section 21.

**25.8.4** Selection of appropriate reagents and standards is included in Section 9 and 22.

**25.8.5** A discussion on selectivity of the test is included in Section 5.

**25.8.6** Constant and consistent test conditions are discussed in Section 19.

**25.8.7** The laboratories sample acceptance policy is included in Section 24.

**25.8.8** A listing of the type of test result correlations that are looked at during report review (e.g. Total Chromium should be greater or equal to Hexavalent Chromium) is included in Section 20.13.4.5.

## SECTION 26.0

### REPORTING RESULTS (NELAC 5.5.10)

#### 26.1 OVERVIEW

The results of each test are reported accurately, clearly, unambiguously, and objectively in accordance with State and Federal regulations as well as client requirements. Analytical results are issued in a format that is intended to satisfy customer and laboratory accreditation requirements as well as provide the end user with the information needed to properly evaluate the results. Where there is a conflict between the client requested formats and accreditation requirements or data usability information, accreditation requirements and data usability information will take precedence over client requests. A variety of report formats are available to meet specific needs.

In cases where a client asks for simplified reports, there must be a written request from the client. There still must be enough information that would show any analyses that were out of conformance (QC out of limits) and there should be a reference to a full report that is made available to the client.

Review of reported data is included in Section 20.

#### 26.2 TEST REPORTS

Analytical results are reported in a format that is satisfactory to the client and meets all requirements of applicable accrediting authorities and agencies. A variety of report formats are available to meet specific needs. The report is printed on laboratory letterhead, reviewed, and signed by the appropriate project manager. At a minimum, the standard laboratory report shall contain the following information:

**26.2.1** A report title (e.g. Analytical Report For Samples) with a “sample results” column header.

**26.2.2** Each report page printed includes the laboratory name, address and telephone number.

**26.2.3** A unique identification of the report (e.g. Lot ID) is on each page along with an identification in order to ensure the page is recognized as part of the report and a clear identification of the end.

**Note:** Page numbers of reports are represented as page # of ##, where the first number is the page number and the second is the total number of pages. Pagination starts at the cover page.

**26.2.4** A copy of the chain of custody (COC).

- Any COCs involved with Subcontracting are included.
- In most cases, the applicable COC is not paginated but is an integral part of the report. If the COC is not a paginated portion of the report then there will be a statement on the front of the report to effect of “The Chain of Custody, X page(s), is included and is an integral part of this report.”
- Any additional addenda to the report must be treated in a similar fashion so it is a recognizable part of the report and cannot accidentally get separated from the report (e.g. Sampling information).

**26.2.5** The name and address of client and a project name/number, if applicable.

**26.2.6** Client project manager or other contact.

**26.2.7** Description and unambiguous identification of the tested sample(s) including the client identification code.

**26.2.8** Date of receipt of sample, date and time of collection, and date(s) of test preparation and performance, and time of preparation or analysis if the required holding time for either activity is less than or equal to 72 hours.

**26.2.9** Date reported or date of revision, if applicable.

**26.2.10** Method of analysis including method code (EPA, Standard Methods, etc).

**26.2.11** Reporting limits.

**26.2.12** Method detection limits (if requested).

**26.2.13** Definition of Data qualifiers and reporting acronyms (e.g. ND).

**26.2.14** Sample results.

**26.2.15** QC data consisting of method blank, surrogate, LCS, and MS/MSD recoveries and control limits.

**26.2.16** Condition of samples at receipt including temperature. This may be accomplished in a narrative or by attaching sample login sheets (Refer to Section 26.2.4 – Item 3 regarding additional addenda).

**26.2.17** A statement to the effect that the results relate only to the items tested and the sample as received by the laboratory.

**26.2.18** A statement that the report shall not be reproduced except in full, without prior express written approval by the laboratory coordinator.

**26.2.19** A signature and title of the person(s) accepting responsibility for the content of the report and date of issue. Signatories are appointed by the Lab Director.

**26.2.20** When NELAC accreditation is required, the lab shall certify that the test results meet all requirements of NELAC or provide reasons and/or justification if they do not.

**26.2.21** The laboratory includes a cover letter.

**26.2.22** Where applicable, a narrative to the report that explains the issue(s) and corrective action(s) taken in the event that a specific accreditation or certification requirement was not met.

**26.2.23** When Soil samples are analyzed, a specific identification as to whether soils are reported on a "wet weight" or "dry weight" basis.

**26.2.24** Appropriate laboratory certification number for the state of origin of the sample, if applicable.

**26.2.25** If only part of the report is provided to the client (client requests some results before all of it is complete), it must be clearly indicated on the report (e.g., partial report, or preliminary report), and that a complete report will follow once all of the work has been completed.

**26.2.26** Any out of network subcontracted analysis results are provided as a separate report on the official letterhead of the subcontractor. All in-network subcontracting is clearly identified on the report as to which laboratory performed a specific analysis.

### **26.3 REPORTING LEVEL OR REPORT TYPE**

TestAmerica West Sacramento offers three levels of quality control reporting. Each level, in addition to its own specific requirements, contains all the information provided in the preceding level. The packages provide the following information in addition to the information described above:

- Level II is a report with the features described in Section 26.2 above, plus quality control sample information, including results for the method blank, percent recovery for laboratory control samples and matrix spike samples, and the RPD values for all MSD and sample duplicate analyses.
- Level III contains all the information supplied in Level II and relevant calibration information, provided on CLP-Like forms or instrument print-outs. No raw data is provided unless it is necessary to provide the relevant calibration information.
- Level IV is the same as Level III with the addition of all raw supporting data.

In addition to the various levels of QC packaging, the laboratory also provides reports in electronic deliverable form, either via e-mail or CD ROM. Initial reports may be provided to clients by facsimile. All faxed reports are followed by hardcopy. Procedures used to ensure client confidentiality are outlined in Section 26.7.

### **26.3.1 Electronic Data Deliverables (EDDs)**

EDDs are routinely offered as part of TestAmerica's services. TestAmerica West Sacramento offers a variety of EDD formats including Environmental Restoration Information Management System (ERPIMS), New Agency Standard (NAS), Format A, Excel, Dbase, GISKEY, SEDD, and Text Files.

EDD specifications are submitted to the IT department by the PM for review and undergo the contract review process. Once the facility has committed to providing data in a specific electronic format, the coding of the format may need to be performed. This coding is documented and validated. The validation of the code is retained by the IT staff coding the EDD.

EDDs shall be subject to a review to ensure their accuracy and completeness. If EDD generation is automated, review may be reduced to periodic screening if the laboratory can demonstrate that it can routinely generate that EDD without errors. Any revisions to the EDD format must be reviewed until it is demonstrated that it can routinely be generated without errors. If the EDD can be reproduced accurately and if all subsequent EDDs can be produced error-free, each EDD does not necessarily require a review.

### **26.4 SUPPLEMENTAL INFORMATION FOR TEST**

The lab identifies any unacceptable QC analyses or any other unusual circumstances or observations such as environmental conditions and any non-standard conditions that may have affected the quality of a result. This is typically in the form of a footnote or a qualifier and/or a narrative explaining the discrepancy in the front of the report. Refer to Appendix 7 for a list of the laboratory's standard footnotes and qualifiers.

**26.4.1** Numeric results with values outside of the calibration range, either high or low are qualified as 'estimated'.

**26.4.2** Where quality system requirements are not met, a statement of compliance/non-compliance with requirements and/or specifications, including identification of test results derived from any sample that did not meet NELAC sample acceptance requirements such as improper container, holding time, or temperature.

**26.4.3** Where applicable, a statement on the estimated uncertainty of measurements; information on uncertainty is needed when a client's instructions so require.

**26.4.4** Opinions and Interpretations - The test report contains objective information, and generally does not contain subjective information such as opinions and interpretations. If such information is required by the client, the Laboratory Director will determine if a response can be prepared. If so, the Laboratory Director will designate the appropriate member of the management team to prepare a response. The response will be fully documented, and reviewed by the Laboratory Director, before release to the client. There may be additional fees charged to the client at this time, as this is a non-routine function of the laboratory.

**Note:** Review of data deliverable packages for submittal to regulatory authorities requires responses to non-conforming data concerning potential impact on data quality. This

necessitates a limited scope of interpretation, and this work is performed by the QA Department. This is the only form of "interpretation" of data that is routinely performed by the laboratory.

When opinions or interpretations are included in the report, the laboratory provides an explanation as to the basis upon which the opinions and interpretations have been made. Opinions and interpretations are clearly noted as such and where applicable, a comment should be added suggesting that the client verify the opinion or interpretation with their regulator.

## **26.5 ENVIRONMENTAL TESTING OBTAINED FROM SUBCONTRACTORS**

If TestAmerica West Sacramento is not able to provide the client the requested analysis, the samples would be subcontracted following the procedures outlined in Section 8.

Data reported from analyses performed by a subcontractor laboratory are clearly identified as such on the analytical report provided to the client. Results from a subcontract laboratory outside of the TestAmerica network are reported to the client on the subcontract laboratory's original report stationary and the report includes any accompanying documentation.

## **26.6 CLIENT CONFIDENTIALITY**

In situations involving the transmission of environmental test results by telephone, facsimile or other electronic means, client confidentiality must be maintained.

TestAmerica will not intentionally divulge to any person (other than the Client or any other person designated by the Client in writing) any information regarding the services provided by TestAmerica or any information disclosed to TestAmerica by the Client. Furthermore, information known to be potentially endangering to national security or an entity's proprietary rights will not be released.

**Note:** This shall not apply to the extent that the information is required to be disclosed by TestAmerica under the compulsion of legal process. TestAmerica will, to the extent feasible, provide reasonable notice to the client before disclosing the information.

**Note:** Authorized representatives of an accrediting authority are permitted to make copies of any analyses or records relevant to the accreditation process, and copies may be removed from the laboratory for purposes of assessment.

**26.6.1** Report deliverable formats are discussed with each new client. If a client requests that reports be faxed or e-mailed, the reports are faxed with a cover sheet or e-mailed with the following note that includes a confidentiality statement similar to the following:

*This material is intended only for the use of the individual(s) or entity to whom it is addressed, and may contain information that is privileged and confidential. If you are not the intended recipient, or the employee or agent responsible for delivering this material to the intended recipient, you are hereby notified that any dissemination, distribution or copying of this communication is strictly prohibited. If you have received this communication in error, please notify us immediately by telephone at (916) 373-5600 (or for e-mails: please notify us immediately by e-mail or by phone (916) 373-5600) and delete this material from any computer.*

## **26.7 FORMAT OF REPORTS**

The format of reports are designed to accommodate each type of environmental test carried out and to minimize the possibility of misunderstanding or misuse.

## **26.8 AMENDMENTS TO TEST REPORTS**

Corrections, additions, or deletions to reports are only made when justification arises through supplemental documentation. Justification is documented using the laboratory's corrective action system (refer to Section 13).

The revised report is retained on the Archive data server, as is the original report. The revised report is stored in the Archive data server under the sample number followed by "Amend". The revised report will have the word "revised" or "amended" and the date in the footer with the pagination.

When the report is re-issued, a notation of "Amended" is placed on the cover/signature page of the report *or at the top of the narrative page* with a brief explanation of reason for the re-issue and a reference back to the last final report generated. For Example: Report was revised on 11/3/07 to include toluene in sample NQA1504 per client's request. This final report replaces the final report generated on 10/27/07.

## **26.9 POLICIES ON CLIENT REQUESTS FOR AMENDMENTS**

### **26.9.1 Sample Reanalysis Policy**

Because there is a certain level of uncertainty with any analytical measurement a sample reanalysis may result in either a higher or lower value from an initial sample analysis. There are also variables that may be present (e.g. sample homogeneity, analyte precipitation over time, etc.) that may affect the results of a reanalysis. Based on the above comments, the laboratory will reanalyze samples at a client's request with the following caveats. Client specific arrangements for reanalysis protocols can be established.

- Homogenous samples: If a reanalysis agrees with the original result to within the RPD limits for MS/MSD or Duplicate analyses, or within  $\pm 1$  reporting limit for samples  $\leq 5x$  the reporting limit, the original analysis will be reported. At the client's request, both results may be reported on the same report but not on two separate reports.
- If the reanalysis does not agree (as defined above) with the original result, then the laboratory will investigate the discrepancy and reanalyze the sample a third time for confirmation if sufficient sample is available.
- Any potential charges related to reanalysis are discussed in the contract terms and conditions or discussed at the time of the request. The client will typically be charged for reanalysis unless it is determined that the lab was in error.
- Due to the potential for increased variability, reanalysis may not be applicable to Non-homogenous, Encore, and Sodium Bisulfate preserved samples. Contact the Department Manager or Laboratory Director if unsure.

### **26.9.2 Policy on Data Omissions or Reporting Limit Increases**

Fundamentally, our policy is simply to not omit previously reported results (including data qualifiers) or to not raise reporting limits and report sample results as ND. This policy has few exceptions. Exceptions are:

- Laboratory error.
- Sample identification is indeterminate (confusion between COC and sample labels).
- An incorrect analysis (not analyte) was requested (e.g., COC lists 8315 but client wanted 8310). A written request for the change is required.
- Incorrect limits reported based on regulatory requirements.
- The requested change has absolutely no possible impact on the interpretation of the analytical results and there is no possibility of the change being interpreted as misrepresentation by anyone inside or outside of our company.

### **26.9.3 Multiple Reports**

TestAmerica does not issue multiple reports for the same workorder where there is different information on each report (this does not refer to copies of the same report) unless required to meet regulatory needs and approved by QA.

**Appendix 1.**

**TESTAMERICA  
ETHICS POLICY No. CA-L-P-001**

Refer to CA-L-P-001 for complete policy.

**TestAmerica  
EMPLOYEE ETHICS STATEMENT**

*I understand that TestAmerica is committed to ensuring the highest standard of quality and integrity of the data and services provided to our clients. I have read the Ethics Policy of the Company.*

- *With regard to the duties I perform and the data I report in connection with my employment at the Company, I agree that:*
- *I will not intentionally report data values that are inconsistent with the actual values observed or measured.*
- *I will not intentionally report the dates, times, sample or QC identifications, or method citations of data analyses that are not the actual dates, times, sample or QC identifications, or method citations.*
- *I will not intentionally misrepresent another individual's work as my own or represent my own work as someone else's.*
- *I will not intentionally misrepresent any data where data does not meet Method or QC requirements. If it is to be reported, I will report it with all appropriate notes and/or qualifiers; I shall not modify data (either sample or QC data) unless the modification can be technically justified through a measurable analytical process, such as one deemed acceptable to the laboratory's Standard Operating Procedures, Quality Assurance Manual or Technical Director. All such modifications must be clearly and thoroughly documented in the appropriate laboratory notebooks/worksheets and/or raw data and include my initials or signature and date.*
- *I shall not make false statements to, or seek to otherwise deceive, members of Management or their representatives, agents, or clients/customers. I will not, through acts of commission, omission, erasure, or destruction, improperly report measurement standards, quality control data, test results or conclusions.*
- *I shall not compare or disclose results for any Performance Testing (PT) sample, or other similar QA or QC requirements, with any employee of any other laboratory, including any other TestAmerica laboratory, prior to the required submission date of the results to the person, organization, or entity supplying the PT sample.*
- *I shall immediately inform my supervisor or other member of management regarding any intentional or unintentional reporting of my own inauthentic data. Such report shall be given both orally and in writing to the supervisor or other member of management contacted and to the local Quality Assurance Manager. The Quality Assurance Manager will initial and date the information and return a copy to me. I shall not condone any accidental or intentional reporting of inauthentic data by other employees and will immediately report its occurrence. If I have actual knowledge of such acts committed by any other employees, and I do not report such information to designated members of Management, it shall be considered as serious as if I personally committed the offense. Accordingly, in that event, I understand that I may be subject to immediate termination of employment.*
- *I understand that if any supervisor, manager, or representative of TestAmerica management instructs, requests, or directs me to perform any of the aforementioned improper laboratory practices, or if I am in doubt or uncertain as to whether or not such laboratory practices are proper, I will not*

*comply. In fact, I must report such event to all appropriate members of Management including, but not limited to, the Lab Director, all supervisors and managers with direct line reporting relationship between me and the Lab Director, and the local Quality Assurance representative, excluding such individuals who participated in such perceived improper instruction, request, or directive. In addition, I may contact Corporate Quality Assurance / Ethics Compliance Officer(s) for assistance.*

- I understand the critical importance of accurately reporting data, measurements, and results, whether initially requested by a client, or retained by TestAmerica and submitted to a client at a later date, or retained by TestAmerica for subsequent internal use;*
- I will not share the pricing or cost data of Vendors or Suppliers with anyone outside of the TestAmerica family of companies.*
- I shall not accept gifts of a value that would adversely influence judgment.*
- I shall avoid conflicts of interest and report any potential conflicts to the management (e.g. employment or consulting with competitors, clients, or vendors).*
- I shall not participate in unfair competition practices (e.g. slandering competitors, collusion with other labs to restrict others from bidding on projects).*
- I shall not misrepresent certifications and status of certifications to clients or regulators.*
- I shall not intentionally discharge wastes illegally down the drain or onto the ground.*
- I understand that any attempt by management or an employee to circumvent these policies will be subject to disciplinary action.*

*As a TestAmerica employee, I understand that I have the responsibility to conduct myself with integrity in accordance with the ethical standards described in the Ethics Policy. I will also report any information relating to possible kickbacks or violations of the Procurement Integrity Act, or other questionable conduct in the course of sales or purchasing activities. I will not knowingly participate in any such activity and will report any actual or suspected violation of this policy to management.*

*I understand that if my job includes supervisory responsibilities, I shall not instruct, request, or direct any subordinate to perform any laboratory practice which is unethical or improper. Also, I shall not discourage, intimidate, or inhibit an employee who may choose to appropriately appeal my supervisory instruction, request, or directive which the employee perceives to be improper, nor retaliate against those who do.*

*The Ethics Policy has been explained to me by my supervisor or at a training session, and I have had the opportunity to ask questions if I did not understand any part of it. I understand that any violation of this policy subjects me to disciplinary action, which can include termination of my employment. In addition, I understand that any violation of this policy which relates to work under a government contract or subcontract could also subject me to the potential for prosecution under federal law.*

EMPLOYEE SIGNATURE \_\_\_\_\_

Date \_\_\_\_\_

Supervisor/Trainer: \_\_\_\_\_

Date \_\_\_\_\_

Work Instruction No. CA-WI-005

**TestAmerica**  
**CONFIDENTIALITY AND PROPRIETARY INFORMATION AGREEMENT**

TestAmerica and their predecessors, in their businesses, have developed and use commercially valuable technical and non-technical information and to guard the legitimate interests of TestAmerica and its clients, it is necessary to protect certain information as confidential and proprietary.

I, \_\_\_\_\_, understand and acknowledge that during the term of my employment by TestAmerica, I will be privy to and entrusted with certain confidential information and trade secrets of TestAmerica and its clients.

*Confidential information and trade secrets include, but are not limited to: customer and client lists; price lists; marketing and sales strategies and procedures; operational and equipment techniques; standard operating procedures; business plans and systems; quality control procedures and systems; special projects and technological research, including projects, research and reports for any government entity or client; client's plans and processes; client's manner of operation; the trade secrets of clients; client's data; vendor or supplier pricing; employee lists and personal information, and any other records, data, files, drawings, inventions, discoveries, applications, or processes which are not in the public domain.*

I agree as follows:

1. I will not in any way, during the term of my employment, or at any time thereafter, except as authorized in writing by the Legal Department of TestAmerica or the client where client data is involved, disclose to others, use for my own benefit, remove from TestAmerica's premises (except to the extent off-site work is approved by my supervisor), copy or make notes of any confidential information and/or trade secrets of TestAmerica or its clients, excepting only that information which may be public knowledge. Technical and business information of any previous employer or other third party which I may disclose to TestAmerica shall be limited to that which was acquired legitimately and disclosed to me without restriction as to secrecy.
2. I agree that all inventions (whether or not patentable) conceived or made by me during the period of my employment by TestAmerica shall belong to TestAmerica, provided such inventions grow out of my work for TestAmerica and are related to the business of TestAmerica. I agree to disclose and assign such inventions to TestAmerica. In California, this provision shall not apply to any invention which qualifies fully under Section 2870 of the California Labor Code.
3. On termination of my employment from TestAmerica, I will deliver to TestAmerica all documents, records, notes, data, memoranda, files, manuals, equipment and things of any nature which relate in any way to confidential information and/or trade secrets of TestAmerica or its clients and which are in my possession or under my control.
4. I agree that during the period of my employment and for one (1) year from and after the termination (for any reason) of my employment with TestAmerica, I shall not directly or indirectly (without first obtaining the written permission of TestAmerica), recruit for employment, or induce to terminate his or her employment with TestAmerica, any person who is an active employee of TestAmerica on the last day of my employment with TestAmerica.
5. I acknowledge that if I were to breach any provision of this Confidentiality Agreement, money damages will be inadequate, and I hereby agree that TestAmerica shall be entitled, where appropriate, to specific performance and/or injunctive relief (i.e. to require me to comply with this Agreement). I further acknowledge that the willingness of TestAmerica to hire me or to continue my employment constitutes full and adequate consideration for the agreements, and obligations to which I have agreed as set forth in this document.

I have executed this Agreement, intending to be legally bound.

\_\_\_\_\_  
Printed Name


\_\_\_\_\_  
Signature

\_\_\_\_\_  
Date

Work Instruction No. CA-WI-006

Appendix 2.

Example Laboratory Organization Chart

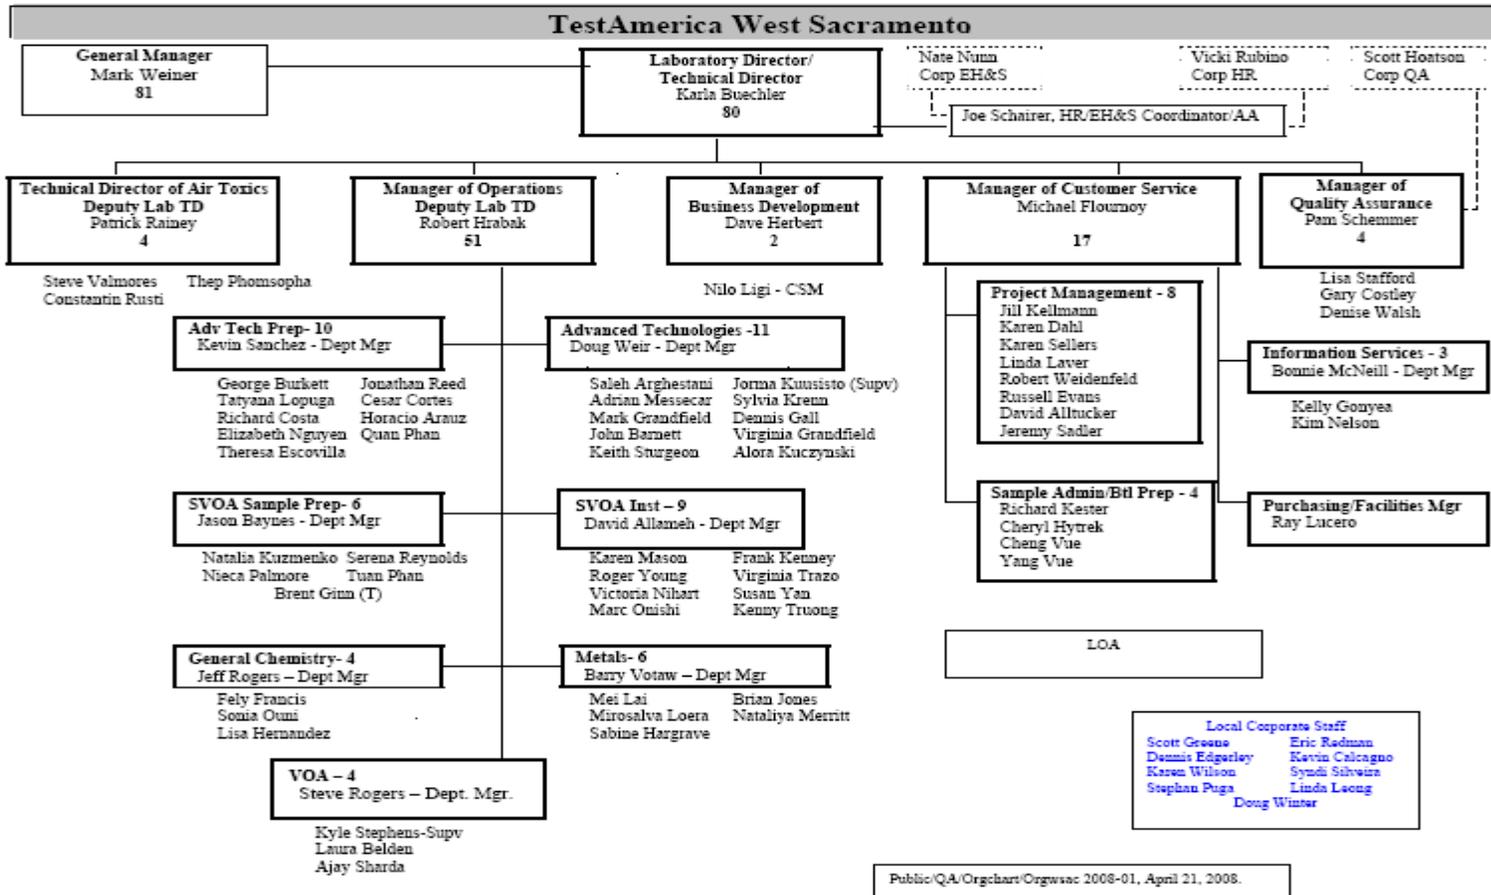

Appendix 3.

Laboratory Floor Plan



Facility Size	Square Feet
Total Area	66,000
Lab Area	43,000
Storage Area	5,200
	Linear Feet
Bench Top	3,000
Hoods	500

**Appendix 4: Listing of Preparation Only Methods Performed**

Method	Aqueous	Solid	Waste	Biological	Air
<b>Organics</b>					
Calif. CAM-WET	X	X	X		
EPA 1311	X	X	X		
EPA 3510C	X				
EPA 3520C	X				
EPA 3535	X				
EPA 3540B		X			
EPA 3542					X
EPA 3550B		X		X	
EPA 3580A			X		
EPA 3600C	X	X	X		
EPA 3620B	X	X	X		
EPA 3630C	X	X	X		
EPA 3640A	X	X		X	
EPA 5030B	X	X	X		
EPA 5035	X	X	X		
<b>Inorganics</b>					
Calif. CAM WET	X	X	X		
EPA 1311	X	X	X		
EPA 1312 (W)	X	X	X		
EPA 3005A	X				
EPA 3010A	X				
EPA 3050B		X	X	X	

**Appendix 4: Listing of Organics Methods Performed**

Parameter	Method	Aqueous	Solid	Waste	Biological	Air
<b>Volatile Organics</b>	SW846 8260B	X	X	X		
<b>Base Neutrals and Acids (BNAs)</b>	SW846 8270B	X	X	X	X	
	TO-13A					X
	IP-7					X
	EPA 23					X
<b>Organochlorine Pesticides</b>	SW846 8081A	X	X	X	X	
	TO-4A					X
	TO-10A					X
	IP-8					X
	WS-ID-0014	X	X	X	X	
<b>PCBs</b>	EPA 8082	X	X	X	X	
	TO-4A					X
	TO-10A					X
<b>Petroleum Hydrocarbons</b>	EPA 8015B	X	X	X		
	CA LUFT	X	X	X		
	AK101	X	X	X		
	Ak102	X	X	X		
	AK103	X	X	X		
	NWTPH-Gx	X	X	X		
	NWTPH-Dx	X	X	X		
	GRO/DRO	X	X	X		
<b>Nitroaromatics and Nitroamines</b>	EPA 8330	X	X	X		X
	EPA 8330A	X	X	X		
	EPA 8330B	X	X	X		
	EPA 8321A (modified)	X	X	X		
	WS-LC-0001	X	X	X		
	WS-LC-0009	X	X	X		
	WS-LC-0010	X	X	X		
<b>PAHs</b>	EPA 8310	X	X	X		
	EPA 8270C (SIM Isotope dilution)	X	X	X	X	X
	EPA 8270C (SIM)	X	X	X		
	CARB 429	X	X	X	X	X
	TO-13A					X
	IP-7					X
<b>Nonly Phenols</b>	WS-LC-0013	X	X		X	
<b>CBSA</b>	WS-LC-0013	X	X			

**Appendix 4: Listing of Organics Methods Performed**

Parameter	Method	Aqueous	Solid	Waste	Biological	Air
<b>Chemical Warfare Degradates</b>	EPA 8321A (Modified)	X	X			
	WS-LC-0004	X	X			
<b>Organosulfur Degradates</b>	EPA 8270C	X	X			
	WS-MS-0003	X	X			
<b>PCB Congeners</b>	EPA 1668A	X	X	X	X	X
<b>Dioxins &amp; Furans</b>	EPA 1613B	X	X			
	EPA 8290	X	X	X	X	
	EPA 8280A	X	X	X	X	
	NCASI 551	X	X			
	DLFM01.1	X	X	X		
	EPA 0023A					X
	EPA 23					X
TO-9					X	

**Appendix 4: Listing of Metals Methods Performed**

Parameter	Methods	Aqueous	Solid	Waste	Biological	Air
<b>Trace Metals</b>	EPA 200.7	X				
	EPA 200.8	X				
	EPA 6010B	X	X	X	X	X
	EPA 6020	X	X	X	X	X
	EPA 0060					X
	EPA 12					X
	CARB 12					X
	EPA 29					X
	CARB 436					X
<b>Hardness</b>	SM 2340B	X				
	EPA 200.7	X				
	EPA 200.8	X				
<b>Mercury</b>	EPA 245.1	X				
	EPA 200.8	X				
	EPA 6020	X				X
	EPA 7470A	X				
	EPA 7471A		X	X	X	X
	EPA 101A					X
	ASTM D6784-02					X
	Ontario-Hydro					X
	EPA 0060					X
	EPA 29					X
	CARB 436					X

**Appendix 4: Listing of Inorganics Methods Performed**

Parameter	Method	Aqueous	Solid	Waste	Biological	Air
<b>Alkalinity (Carbonate, Bicarbonate, Total)</b>	SM 2320B	X				
<b>Ammonia</b>	EPA 350.1	X				
<b>Bromide</b>	EPA 300.0	X				
	EPA 9056	X	X			
	EPA 9057					X
	EPA 26A					X
	CARB 421					X
<b>Carbon, Total Inorganic</b>	EPA 9060	X	X			
<b>Carbon, Total Organic</b>	EPA 9060	X	X			
	SM 5310 C	X				
<b>Chloride</b>	EPA 300.0	X				
	EPA 9056	X	X			
	EPA 9057					X
	EPA 26A					X
	CARB 421					X
<b>Chromium, Hexavalent</b>	EPA 7196A	X	X			
	EPA 0061					X
	EPA 306					X
	CARB 426					X
<b>Conductivity</b>	EPA 9050A	X				
	SM 2510 B	X				
<b>Cyanide, Free</b>	EPA 9012A	X	X			
	SM 4500 CN E	X				
<b>Cyanide, Total</b>	EPA 335.4	X				
	EPA 9012A	X	X			
	CARB 426					X
<b>Demand, Chemical Oxygen</b>	EPA 410.4	X				
<b>Flouride</b>	EPA 300.0	X	X			
	EPA 9056	X	X			
	EPA 9214	X	X			
	SM 4500 F C	X				
	EPA 9057					X
	EPA 26A					X
	CARB 421					X
<b>n-Hexane Extractable Materials</b>	EPA 1664A	X				
	EPA 9070A	X				
	EPA 9071B		X			
<b>Moisture</b>	ASTM 2216		X			

**Appendix 4: Listing of Inorganics Methods Performed**

Parameter	Method	Aqueous	Solid	Waste	Biological	Air
Nitrate	EPA 353.2	X				
	EPA 300.0	X				
	EPA 9056	X	X			
	CARB 421					X
Nitrate-Nitrite	EPA 353.2	X				
Nitrite	EPA 353.2	X				
	EPA 300.0	X				
	EPA 9056	X	X			
	CARB 421					X
Nitrocellulose	EPA 353.2	X	X			
	WS-WC-0050	X	X			
Total Kjeldahl Nitrogen	EPA 351.2	X				
Orthophosphate	EPA 365.3	X				
	EPA 300.0	X				
	EPA 9056	X	X			
Particulates in Air	EPA 5					X
	40 CFR Part 50					X
Perchlorate	EPA 314.0	X				
	EPA 331.0	X				
	EPA 6850	X	X			
	WS-LC-0012	X	X			
pH	SM 4500 H+ B	X				
	EPA 150.2	X				
	EPA 9040A	X				
	EPA 9041A	X				
	EPA 9045C		X	X		
Phenolics	EPA 420.4	X				
	EPA 9066	X	X			
Phosphorus, Total	EPA 365.3	X				
	EPA 365.4	X				
Solids, Total	SM 2540 B	X				
Solids, Total Dissolved	SM 2540 C	X				
Solids, Total Suspended	SM 2540 D	X				
Settleable Solids	SM 2540 F	X				
Sulfate	EPA 300.0	X				
	EPA 9065	X				
Sulfide	SM 4500 S2- D	X				
Turbidity	SM 2130 B	X				

**Appendix 4: Summary of QC for General Chemistry Methods: Titration (Alkalinity), Method SM 2320 B**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	$< \pm$ RL from zero.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within 90-100%.	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within 90-110 %.	If not within laboratory control limits, rerun all associated samples.
<b>Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	RPD $\leq$ 20%.	Reanalyze once, evaluate. Flag data if reanalysis remains out of control outside of limit.
<b>ICAL</b>	Daily, 3 point calibration of pH meter.	$r \geq 0.995$ .	Check buffers, perform instrument maintenance, repeat calibration.
<b>ICV/ICB</b>	Start of every sequence, following ICAL.	$\pm 10\%$ of true value for ICV, $< \pm$ RL from zero for ICB.	Evaluate standards, recalibrate, reanalyze affected samples.
<b>CCV/CCB</b>	Every 10 samples and end of sequence.	$\pm 10\%$ of true value for ICV, $< \pm$ RL from zero for CCB.	Evaluate standards, recalibrate, reanalyze affected samples.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: Colorimetric Methods, EPA 335.2, EPA 350.1, EPA 351.2, EPA 353.3, EPA 365.3, EPA 365.4, EPA 376.2, EPA 410.4, EPA 420.2, EPA 7196A, EPA 9012A, SM 3500 Cr D, SM 4500 CN E, & SM 4500 S2- D**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Refer to Method/SOP.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits; RPD must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	Evaluate MSD.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits; RPD must be within laboratory control limits.	Reanalyze once, evaluate. Flag data if reanalysis remains out of control. (Further action required for Cr6+ analysis, refer to method SOP).
<b>Duplicate</b>	As requested by client or required by specific method. Sometimes not necessary as MSD fulfills the requirement.	RPD must meet method limits.	Flag data outside of limit.
<b>Post-Spike/MSA (CR6+ only)</b>	Minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits	Evaluate acidity; see MSD.
<b>ICAL</b>	Multi-level calibration with blank, daily prior to sample analysis.	$r \geq 0.995$ .	Evaluate data, correct problem, reanalyze.
<b>ICV/ICB</b>	Start of every sequence, following ICAL.	$\pm 10\%$ of true value for ICV, < RL for ICB (1/2 RL for Cyanide).	Evaluate data, correct problem, reanalyze.
<b>CCV/CCB</b>	Every 10 samples and end of analysis.	$\pm 10\%$ of true value for CCV, < RL for CCB (1/2 RL for Cyanide).	Evaluate data; reanalyze affected samples with good CCV/CCB.
<b>Other (Cyanide Methods)</b>	Distill high and low standard with every batch.	$\pm 10\%$ of true value.	Evaluate data, correct problem, reanalyze.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: Ion Chromatography, EPA 300.0, EPA 314.0, EPA 9056, & EPA 26A**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	<RL; (<1/2 RL for 314.0).	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	90-100% recovery (85-115% for 314.0).	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	90-110% recovery (85-115% for 314.0) 15% RPD.	If not within laboratory control limits, rerun all associated samples.
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Aqueous: 80-120% recovery. Soil: 80-120% recovery; (75-125% for 314.0).	Evaluate MSD.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Aqueous: 80-120% recovery; RPD 20% (15% for 314.0). Soil: 80-120% recovery; (75-125% for 314.0); RPD 20%.	Reanalyze once, evaluate. Flag data if reanalysis remains out of control.
<b>Duplicate</b>	As requested by client or required by specific method (1 dup every 10 samples for 9056). Sometimes not necessary as MSD fulfills the requirement.	RPD must meet method limits.	Flag data outside of limit.
<b>ICAL</b>	5 levels plus a blank, repeated monthly or following maintenance.	$r \geq 0.995$ ; (Air methods, before and after sample analysis, pre- and post-must be within $\pm 5\%$ of mean),	Perform instrument maintenance, repeat calibration.
<b>ICV/ICB</b>	Start of every sequence, following ICAL.	$\pm 10\%$ of true value for ICV, < RL for ICB (1/2 RL for 314.0),	Evaluate standards, recalibrate or reanalyze.
<b>CCV/CCB</b>	Every 10 samples and at the end of the analytical sequence.	$\pm 10\%$ of true value for CCV ( $\pm 15\%$ for 314.0); < RL for CCB (1/2 RL for 314.0),	Evaluate standards, recalibrate or reanalyze.
<b>MCT (314.0)</b>	Daily, prior to sample analysis.	$\pm 20\%$ of true value.	Correct problem, recalibrate if needed.
<b>ICCS (314.0)</b>	Daily, prior to sample analysis.	$\pm 25\%$ of true value.	Correct problem, recalibrate if needed.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: Conductivity, EPA 120.1, EPA 9060A, & SM 2510 B**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Refer to Method/SOP.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	RPD must meet method limits.	Flag data outside of limit.
<b>ICAL</b>	1 level to determine cell constant, daily, prior to analysis.		
<b>ICV/ICB</b>	Start of every sequence, following ICAL.	$\pm 10\%$ of true value for ICV, $< \pm RL$ from zero for ICB.	Evaluate standards, recalibrate as needed, reanalyze.
<b>CCV/CCB</b>	Every 10 samples and end of sequence.	$\pm 10\%$ of true value for ICV, $< \pm RL$ from zero for CCB.	Evaluate standards and samples, reanalyze affected samples.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: Ion Specific Electrode, SM 4500 F- & EPA 9214**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	< $\pm$ RL from zero.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be 90 – 100%.	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be 90 – 100%.	If not within laboratory control limits, rerun all associated samples.
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	Evaluate MSD.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits; RPD must be within laboratory control limits.	Reanalyze once, evaluate. Flag data if reanalysis remains out of control.
<b>Duplicate</b>	As requested by client. MSD may fulfill the requirement.	RPD must meet method limits.	Flag data outside of limit.
<b>ICAL</b>	Daily, 6 levels.	$r \geq 0.995$ .	Check standards and probe, replace as needed, recalibrate.
<b>ICV/ICB</b>	Start of every sequence, following ICAL	$\pm 10\%$ of true value for ICV, < $\pm$ RL from zero for ICB.	Check standards and probe, replace as needed, recalibrate.
<b>CCV/CCB</b>	Every 10 samples.	$\pm 10\%$ of true value for ICV, < $\pm$ RL from zero for CCB.	Evaluate date, reanalyze affected samples and CCV.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: pH, EPA 150.2, EPA 9040B, EPA 9045C, & SM 4500 H<sup>+</sup>**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	± 0.1 pH unit.	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	± 0.1 pH unit.	If not within laboratory control limits, rerun all associated samples.
<b>Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Agree within ± 0.1 pH unit.	Flag data outside of limit.
<b>ICAL</b>	Daily. <u>Meter</u> : 2 level calibration that bracket the expected pH of the sample; <u>Autoanalyzer</u> : 3 levels at pH 4, 7, and 10.	± 0.05 pH units of true value (meter), r ≥ 0.995 (autoanalyzer).	Evaluate buffers and probe, replace as needed and recalibrate.
<b>ICV</b>	Daily, prior to sample analysis, single buffer check.	± 0.1 pH unit.	Evaluate buffers and probe, replace as needed and recalibrate.
<b>CCV</b>	Following every 10 samples and at the end of the run.	± 0.1 pH unit.	Evaluate affected samples, reanalyze affected samples and CCV.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: Total Organic Carbon, EPA 415.1, EPA 9060, & SM 5310 C**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	< RL.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	Evaluate MSD.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits; RPD must be within laboratory control limits.	Reanalyze once, evaluate. Flag data if reanalysis remains out of control.
<b>Duplicate</b>	As requested by client or required by specific method. Sometimes not necessary as MSD fulfills the requirement.	RPD must meet method limits.	Flag data outside of limit.
<b>ICAL</b>	Daily, prior to analysis, 4 levels plus a blank. (5 levels for solid)	$r \geq 0.995$ .	Evaluate standards and instrument, perform maintenance, recalibrate.
<b>ICV/ICB</b>	Start of every sequence, following ICAL.	<u>Aqueous</u> : $\pm 10\%$ of true value for ICV, < RL for ICB. <u>Solid</u> : $\pm 15\%$ of true value for ICV, < RL for ICB.	Evaluate standards and instrument, re-prepare, recalibrate.
<b>CCV/CCB</b>	Every 10 samples.	$\pm 10\%$ of true value for CCV, < RL for CCB.	Evaluate samples, reanalyze affected samples.

Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.

**Appendix 4: Summary of QC for General Chemistry Methods: Turbidity, EPA 180.1, SM 2130 B**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	$< \pm$ RL from zero.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	RPD must be within laboratory control limits.	Flag data outside of limit.
<b>ICAL</b>	Daily, prior to analysis, 4 levels plus a blank.	$r \geq 0.995$	Evaluate instrument and standards, recalibrate.
<b>ICV/ICB</b>	Start of every sequence, following ICAL.	$\pm 10\%$ of true value for ICV, $< \pm$ RL from zero for ICB.	Evaluate instruments and standards, reanalyze, recalibrate.
<b>CCV/CCB</b>	Every 10 samples and end of sequence.	$\pm 10\%$ of true value for CCV, $< \pm$ RL from zero for CCB.	Evaluate affected samples, reanalyze.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: Residue, SM 2540 B, C, D and F**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	< ± RL from zero.	Rerun all samples associated with unacceptable blank
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within 80 – 120%.	If not within laboratory control limits, rerun all associated samples
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within 80 – 120%, RPD ≤ 20%.	If not within laboratory control limits, rerun all associated samples
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within 85 – 115%.	Evaluate MSD.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within 85 – 115%, RPD ≤ 20%.	Reanalyze once, evaluate. Flag data if reanalysis remains out of control.
<b>Duplicate</b>	As requested by client or required by specific method.	RPD ≤ 20% for samples > 5x RL.	Flag data outside of limit.
<b>Balance Calibration Check</b>	Daily, before use, with weights bracketing the masses to be measured.	Refer to SOP WS-QA-0041.	Have balance serviced.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for General Chemistry Methods: Oil & Grease, EPA 1664A, EPA 9070, & EPA 9071B**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Refer to Method/SOP	Rerun all samples associated with unacceptable blank
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits	If not within laboratory control limits, rerun all associated samples
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits	If not within laboratory control limits, rerun all associated samples
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits	Evaluate MSD.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits; RPD must be within laboratory control limits	Reanalyze once, evaluate. Flag data if reanalysis remains out of control. (Further action required for Cr6+ analysis, see SOP SAC-WC-0020).
<b>Balance Calibration Check</b>	Daily, before use, with weights bracketing the masses to be measured. Additionally, with 2 and 1000 mg weights.	Refer to SOP WS-QA-0041 for daily check. <u>HEM Specific:</u> 1.8 – 2.2 mg and 995-1005 mg.	Have balance serviced.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for Metals Methods: Mercury, EPA 245.1, EPA 7470A, & EPA 7471A**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Concentration less than reporting limit.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Rerun all samples associated with unacceptable LCS.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MS.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MSD.
<b>ICAL</b>	As needed, 5 levels plus blank (ICAL is digested with samples).	$r \geq 0.995$ .	Evaluate instrument and standards, re-digest calibration and repeat.
<b>ICV/ICB</b>	Following ICAL, prior to sample analysis.	<u>245.1:</u> ICV $\pm$ 5% of true value, ICB $< \pm$ RL <u>7470/7471:</u> ICV $\pm$ 10% of true value, ICB $< \pm$ RL	Evaluate standards, remake/redigest as needed.
<b>CCV/CCB</b>	Every 10 samples and end of run.	<u>245.1:</u> CCV $\pm$ 10% of true value, CCB $< \pm$ RL <u>7470/7471:</u> CCV $\pm$ 20% of true value, CCB $< \pm$ RL	Evaluate affected samples, reanalyze samples and standards.
<b>IDLs</b>	Annually.		

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for Metals Methods: Trace Metals, EPA 200.7, EPA 200.8, EPA 6010B, and EPA 6020**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Concentration less than reporting limit.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Rerun all samples associated with unacceptable LCS.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed	Percent recovery must be within laboratory control limits.	If not within laboratory control limits, rerun all associated samples.
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MS.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MSD.
<b>Post-digestion Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Dilute and reanalyze.
<b>Serial Dilution</b>	1 with each batch of samples processed not to exceed 20 samples.	± 10% Difference.	Flag data associated with unacceptable Serial Dilution, no further action unless client specified.
<b>ICAL</b>	Daily, As needed, 1 level and blank.	Rerun high calibration standard: verify quantitation at ± 5% of true value	Evaluate standards and instrument, perform maintenance, recalibrate.
<b>ICV/ICB</b>	Following ICAL, prior to samples.	<u>200.7</u> : ICV ± 5% of true value <u>200.8 / 6010 /6020</u> : ICV ± 10% <u>200.7 / 6010</u> : ICV RSD < 5% from replicate; <u>All</u> : ICB < RL.	Evaluate standards.
<b>CCV/CCB</b>	Every 10 samples and end of run.	± 10% of true value; CCV RSD < 5% from replicate (ICP); CCB < RL.	Evaluate standards and samples, reanalyze affected samples.
<b>ICSA/ICSAB</b>	Analyze at beginning of run.	Refer to laboratory SOP.	
<b>Initial Tuning (ICPMS only)</b>	Before instrument is brought on-line, then as needed.	Initial tuning standard deviation ≤ 5% for four replicates; Mass calibration ≤ 0.1 amu from true; Resolution ≤ 0.75 amu full width at 5% peak height.	Perform maintenance and repeat.
<b>Interelement Correction Factors (ICP only)</b>	Semi-annually.		
<b>IDLs</b>	Annually (ICP) Semi-Annually (ICPMS)		

Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.

**Appendix 4: Summary of QC for Organics Methods: GC/LC, EPA 8015B, EPA 8081A, EPA 8082, EPA 8310, EPA 8330, NWTPH-Dx, CA-LUFT, AK102, AK103, TO-4A, Ws-LC-0010**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Concentration less than reporting limit	Rerun all samples associated with unacceptable blank
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits	Rerun all samples associated with unacceptable LCS
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory control limits	If not within laboratory control limits, rerun all associated samples
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits	Flag data associated with unacceptable MS.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits	Flag data associated with unacceptable MSD
<b>Surrogates (QC Samples)</b>	Surrogates are spiked into method blank and all samples (QC included).	Percent recovery must be within laboratory (or method, as applicable) control limits	All surrogates must be within laboratory established control limits before sample analysis may proceed.
<b>Surrogates (Field Samples)</b>	Surrogates are spiked into method blank and all samples (QC included).	Percent recovery must be within laboratory (or method, as applicable) control limits	Reprepare and reanalyze samples or flag sample data not meeting surrogate criteria
<b>ICAL</b>	As needed, minimum of 5 levels. See method SOP for multi-eluting compounds.	Average RF $\leq$ 20%, or linear regression $r \leq$ 0.995, or non-linear regression COD $<$ 0.990, intercepts $\leq$ $\frac{1}{2}$ RL	Perform maintenance, reanalyze.
<b>ICV</b>	Second source mid-point standard run immediately following ICAL.	All components % drift $\leq$ method criteria.	Evaluate ICAL and ICV standards
<b>CCV</b>	Midpoint calibration standard following every 10 samples (or other interval as specified in method/SOP) and end of run.	All components % drift $\leq$ method criteria.	Stop analysis sequence, perform any needed maintenance, reanalyze CCV and affected samples.
<b>PEM (8081A)</b>	With ICAL, once every 12 hours during analysis.	% breakdown (DDT, Endrin) $<$ 15%.	Stop analysis sequence, perform any needed maintenance, reanalyze PEM and affected samples.
<b>RT Window Mixture (Hydrocarbons)</b>	With ICAL, more frequently as required by specific method.	Refer to Method SOP.	

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for Organics Methods: GCMS Internal Standard, EPA 521, EPA 8260, EPA 8270, EPA TO-13A, EPA IP-7, CA-LUFT, NWTPH-Gx, AK 101, WS-MS-0003, WS-MS-0009, & WS-MS-0010 (Alkyl phenols)**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Concentration less than reporting limit	Rerun all samples associated with unacceptable blank
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Rerun all samples associated with unacceptable LCS
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	If not within laboratory control limits, rerun all associated samples
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MS.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MSD
<b>Duplicate (EPA 521)</b>	1 per 20 samples, minimum of one per batch of samples processed. (May substitute MSD if samples routinely ND)	RPD must be within method control limits.	Flag data associated with unacceptable duplicate
<b>Surrogates (QC Samples)</b>	In each QC sample.	Percent recovery must be within laboratory (or method, as applicable) control limits.	All surrogates must be within laboratory established control limits before sample analysis may proceed.
<b>Surrogates (Field Samples)</b>	In each field (client-submitted) sample.	Percent recovery must be within laboratory (or method, as applicable) control limits	Reprepare and reanalyze samples or flag sample data not meeting surrogate criteria
<b>Internal Standards</b>	Internal Standards are added to all samples (QC samples included).	Refer to Method SOP.	Evaluate data and instrument. If no instrument issue found, flag data.
<b>ICAL</b>	Minimum of 5 levels, As needed.	Refer to Method SOP.	Perform maintenance, reanalyze.
<b>ICV</b>	Mid-level second source standard immediately following calibration curve.	Refer to Method SOP.	Evaluate ICAL and ICV standards.
<b>CCV</b>	Mid-level standard every 12 hours (after tuning), prior to sample analysis. <u>TPH only:</u> At end of run.	Refer to Method SOP.	Evaluate instrument, perform maintenance as needed. Reanalyze affected samples.
<b>Tuning Check (Full Scan Methods)</b>	BFB or DFTPP tuning at the beginning of every shift, (as defined in method SOP) including before ICALs	Refer to Method SOP.	Evaluate instrument and reanalyze. Perform maintenance as needed.
<b>Tuning Check SIM Methods</b>	"Autotune" function of instrument.	Refer to Method SOP.	Evaluate instrument and reanalyze. Perform maintenance as needed.
<b>RT Window Mixture (Hydrocarbons)</b>	Every ICAL, more frequently as required by reference method.	Refer to method SOP.	

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for Organics Methods: GCMS Isotope Dilution: EPA 535, EPA 1613B, EPA 1625 (modified), EPA 1668A, EPA 8280A, EPA 8290, EPA TO-9, EPA 23, EPA 0023A, PAH SIM Isotope Dilution**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Concentration less than reporting limit	Rerun all samples associated with unacceptable blank
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Rerun all samples associated with unacceptable LCS
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	If not within laboratory control limits, rerun all associated samples
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MS.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MSD
<b>Internal Standards</b>	Labeled Isotopes are added to all samples (QC samples included).	Percent recovery must be within method control limits.	Evaluate data. Re-extract.
<b>Cleanup Standards</b>	Labeled Isotopes are added to all samples (QC samples included), as specified by source method.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Evaluate data. Re-extract.
<b>Mass Resolution Check</b>	Prior to analysis, end of analysis as defined by method SOP.	Refer to Method SOP.	Evaluate data, perform maintenance and reanalyze if adverse impact.
<b>ICAL</b>	5 levels (+ window defining solution, if applicable).	% RSD ≤ method criteria, ion ratios meet method criteria.	Perform maintenance, reanalyze.
<b>ICV</b>	Second source mid-point stand run following ICAL.	RFs with %D ≤ from ICAL within method/SOP criteria	Evaluate ICAL and ICV standards.
<b>CCV</b>	1 level every 12 hours after window performance mix (if applicable to method)	Refer to Method SOP	Evaluate instrument, perform maintenance as needed. Reanalyze affected samples.
<b>Ending</b>	See Method SOP, not applicable to all methods.	Refer to Method SOP.	Evaluate instrument, perform maintenance as needed. Reanalyze affected samples.
<b>Window Performance Mix</b>	Method specific, refer to method SOP.	Refer to Method SOP.	Evaluate instrument, perform maintenance as needed. Recalibrate and reanalyze affected samples.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for Organics Methods: LCMS , EPA 8321A (Modified), WS-LC-0013, WS-LC-0001, & WS-LC-0004**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Concentration less than reporting limit	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits	Rerun all samples associated with unacceptable LCS.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits	If not within laboratory control limits, rerun all associated samples.
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits	Flag data associated with unacceptable MS.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits	Flag data associated with unacceptable MSD.
<b>Surrogates (QC Samples)</b>	When available, surrogates are spiked into method blank and all samples (QC included).	Percent recovery must be within laboratory (or method, as applicable) control limits	All surrogates must be within laboratory established control limits before sample analysis may proceed.
<b>Surrogates (Field Samples)</b>	When available, surrogates are spiked into method blank and all samples (QC included).	Percent recovery must be within laboratory (or method, as applicable) control limits	Reprepare and reanalyze samples or flag sample data not meeting surrogate criteria.
<b>Tune</b>	Performed by service engineer following major maintenance.	Manufacturer's specifications.	Continue maintenance.
<b>Mass Calibration</b>	As needed	m/z within 0.3 amu of expected value.	Repeat until adequate signals obtained.
<b>ICAL</b>	As needed.	RSD $\leq$ method/SOP criteria, regression lines $r^2 \geq 0.990$ , intercept $< \frac{1}{2}$ RL.	If RSD, $r^2$ or intercept not met, perform instrument maintenance and recalibrate.
<b>ICV</b>	Second source mid-point stand run following ICAL.	All %drift $\leq$ method/SOP criteria	Evaluate standards.
<b>MRL</b>	Low-level standard, as required by method/program.	All %drift $\leq$ method/SOP/program criteria	Evaluate impact, reanalyze affected samples and standards.
<b>CCV</b>	Midpoint calibration standard following every 10 samples and end of run.	All %drift $\leq$ method/SOP criteria	Evaluate impact, reanalyze affected samples and standards.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

**Appendix 4: Summary of QC for Organics Methods: LCMS Isotope Dilution, EPA 331, EPA 6850, WS-LC-0012, & WS-LC-0020**

QC Check	Frequency	Acceptance Criteria	Corrective Action
<b>Method Blank</b>	1 per 20 samples, minimum of one per batch of samples processed.	Concentration less than reporting limit.	Rerun all samples associated with unacceptable blank.
<b>Laboratory Control Sample</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Rerun all samples associated with unacceptable LCS.
<b>Laboratory Control Sample Duplicate</b> <i>(if required by client/program)</i>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	If not within laboratory control limits, rerun all associated samples
<b>Matrix Spike</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MS.
<b>Matrix Spike Duplicate</b>	1 per 20 samples, minimum of one per batch of samples processed.	Percent recovery & RPD must be within laboratory (or method, as applicable) control limits.	Flag data associated with unacceptable MSD.
<b>Internal Standards</b>	Labeled Isotopes are added to all samples (QC samples included).	Percent recovery must be within laboratory (or method, as applicable) control limits	Evaluate data. Re-extract.
<b>Tune</b>	Performed by service engineer following major maintenance.	Manufacturer's specifications.	Continue maintenance.
<b>Mass Calibration</b>	As needed	m/z within 0.3 amu of expected value, or other criteria as specified by method.	Repeat until adequate signals obtained.
<b>ICAL</b>	As needed.	RSD $\leq$ method/SOP criteria, regression lines $r^2 \geq 0.990$ , intercept $< \frac{1}{2}$ RL/IS.	If RSD, $r^2$ or intercept not met, perform instrument maintenance and recalibrate.
<b>ICV</b>	Second source mid-point stand run following ICAL.	All %drift $\leq$ method/SOP criteria	Evaluate standards.
<b>MRL</b>	Low-level standard, as required by method/program.	All %drift $\leq$ method/SOP/program criteria	Evaluate impact, reanalyze affected samples and standards.
<b>CCV</b>	Midpoint calibration standard following every 10 samples and end of run.	All %drift $\leq$ method/SOP criteria	Evaluate impact, reanalyze affected samples and standards.

*Note: Refer to the analysis method/laboratory SOP for specific QC requirements. Not all QC samples listed here are required for all methods.*

## **Appendix 5. Glossary/Acronyms**

### **Glossary:**

#### Acceptance Criteria:

Specified limits placed on characteristics of an item, process, or service defined in requirement documents. (ASQC)

#### Accreditation:

The process by which an agency or organization evaluates and recognizes a laboratory as meeting certain predetermined qualifications or standards, thereby accrediting the laboratory. In the context of the National Environmental Laboratory Accreditation Program (NELAP), this process is a voluntary one. (NELAC)

#### Accrediting Authority:

The Territorial, State, or Federal Agency having responsibility and accountability for environmental laboratory accreditation and which grants accreditation (NELAC) [1.5.2.3]

#### Accuracy:

The degree of agreement between an observed value and an accepted reference value. Accuracy includes a combination of random error (precision) and systematic error (bias) components which are due to sampling and analytical operations; a data quality indicator. (QAMS)

#### Analyst:

The designated individual who performs the “hands-on” analytical methods and associated techniques and who is the one responsible for applying required laboratory practices and other pertinent quality controls to meet the required level of quality. (NELAC)

#### Assessment:

The evaluation process used to measure or establish the performance, effectiveness, and conformance of an organization and/or its systems to defined criteria (to the standards and requirements of NELAC). (NELAC)

#### Assessment Criteria:

The measures established by NELAC and applied in establishing the extent to which an applicant is in conformance with NELAC requirements. (NELAC)

#### Assessment Team:

The group of people authorized to perform the on-site inspection and proficiency testing data evaluation required to establish whether an applicant meets the criteria for NELAP accreditation. (NELAC)

**Assessor:**

One who performs on-site assessments of accrediting authorities and laboratories' capability and capacity for meeting NELAC requirements by examining the records and other physical evidence for each one of the tests for which accreditation has been requested. (NELAC)

**Audit:**

A systematic evaluation to determine the conformance to quantitative and qualitative specifications of some operational function or activity. (EPA-QAD)

**Batch:**

Environmental samples which are prepared and/or analyzed together with the same process and personnel, using the same lot(s) of reagents. A preparation batch is composed of one to 20 environmental samples of the same matrix, meeting the above mentioned criteria and with a maximum time between the start of processing of the first and last sample in the batch to be 24 hours. An analytical batch is composed of prepared environmental samples (extracts, digestates or concentrates) and /or those samples not requiring preparation, which are analyzed together as a group using the same calibration curve or factor. An analytical batch can include samples originating from various environmental matrices and can exceed 20 samples. (NELAC Quality Systems Committee)

**Bias:**

A systematic (consistent) error in test results. Bias is expressed as the difference between the population mean and the true or reference value, or as estimated from sample statistics, the difference between the sample average and the reference value.

**Blank:**

A sample that has not been exposed to the analyzed sample stream in order to monitor contamination during sampling, transport, storage or analysis. The blank is subjected to the usual analytical and measurement process to establish a zero baseline or background value and is sometimes used to adjust or correct routine analytical results. (ASQC)

**Blind Sample:**

A sample for analysis with a composition known to the submitter. The analyst/laboratory may know the identity of the sample but not its composition. It is used to test the analyst's or laboratory's proficiency in the execution of the measurement process.

**Calibration:**

To determine, by measurement or comparison with a standard, the correct value of each scale reading on a meter, instrument, or other device. The levels of the applied calibration standard should bracket the range of planned or expected sample measurements. (NELAC)

**Calibration Curve:**

The graphical relationship between the known values, such as concentrations, of a series of calibration standards and their instrument response. (NELAC)

**Calibration Method:**

A defined technical procedure for performing a calibration. (NELAC)

**Calibration Standard:**

A substance or reference material used to calibrate an instrument (QAMS)

**Certified Reference Material (CRM):**

A reference material one or more of whose property values are certified by a technically valid procedure, accompanied by or traceable to a certificate or other documentation which is issued by a certifying body. (ISO Guide 30-2.2)

**Chain of Custody:**

An unbroken trail of accountability that ensures the physical security of samples and includes the signatures of all who handle the samples. (NELAC) [5.12.4]

**Clean Air Act:**

The enabling legislation in 42 U.S.C. 7401 et seq., Public Law 91-604, 84 Stat. 1676 Pub. L. 95-95, 91 Stat., 685 and Pub. L. 95-190, 91 Stat., 1399, as amended, empowering EPA to promulgate air quality standards, monitor and enforce them. (NELAC)

**Comparability:**

Comparability is a measure of the confidence with which one data set can be compared to another. To ensure comparability, all laboratory analysts are required to use uniform procedures (i.e., SOPs) and a uniform set of units and calculations for analyzing and reporting environmental data.

**Completeness:**

Completeness is a measure of the percentage of measurements that are judged to be valid measurements. At a minimum, the objective for completeness of data is 90% for each constituent analyzed. It is usually expressed as a percentage of the total number of measurements.

**Composite:**

A sample composed of two or more increments.

**Comprehensive Environmental Response, Compensation and Liability Act (CERCLA/SUPERFUND):**

The enabling legislation in 42 U.S.C. 9601-9675 et seq., as amended by the Superfund Amendments and Reauthorization Act of 1986 (SARA), 42 U.S.C. 9601 et seq., to eliminate the health and environmental threats posed by hazardous waste sites. (NELAC)

**Compromised Samples:**

Those samples which are improperly sampled, insufficiently documented (chain of custody and other sample records and/or labels), improperly preserved, collected in improper containers, or exceeding holding times when delivered to a laboratory. Under normal conditions,

compromised samples are not analyzed. If emergency situation require analysis, the results must be appropriately qualified. (NELAC)

**Confidential Business Information (CBI):**

Information that an organization designates as having the potential of providing a competitor with inappropriate insight into its management, operation or products. NELAC and its representatives agree to safeguarding identified CBI and to maintain all information identified as such in full confidentiality.

**Confirmation:**

Verification of the identity of a component through the use of an approach with a different scientific principle from the original method. These may include, but are not limited to:

- Second column confirmation
- Alternate wavelength
- Derivatization
- Mass spectral interpretation
- Alternative detectors or
- Additional Cleanup procedures

(NELAC)

**Conformance:**

An affirmative indication or judgement that a product or service has met the requirements of the relevant specifications, contract, or regulation; also the state of meeting the requirements. (ANSI/ASQC E4-1994)

**Control Chart:**

A graphical representation of analytical accuracy. Displays the arithmetic mean of a data set, the upper and lower warning limits and the upper and lower control limits.

**Corrective Action:**

The action taken to eliminate the causes of an existing nonconformity, defect or other undesirable situation in order to prevent recurrence. (ISO 8402)

**Correlation coefficient**

The correlation coefficient ( $r$ ) is a determination of how closely data "fits" a straight line. It is a number between -1 and 1 that indicates the degree of linear relationship between two sets of numbers. A correlation coefficient of +1 (usually calculated to three decimal places or 1.000) means the data falls exactly on a straight line with positive slope. A correlation coefficient of -1 (or -1.000) means the data falls exactly on a straight line with negative slope.

**Data Audit:**

A qualitative and quantitative evaluation of the documentation and procedures associated with environmental measurements to verify that the resulting data re of acceptable quality (i.e., that they meet specified acceptance criteria). (NELAC)

**Data quality objective (DQO):**

Data quality objectives (DQOs) are qualitative and quantitative statements used to ensure the generation of the type, quantity, and quality of environmental data that will be appropriate for the intended application (EPA 1994). Typically, DQOs are identified during project scope and development of sampling and analysis plans. In this QA manual, however, we refer to only the analytical DQOs because laboratories generally do not have any authority over sample collection, shipment, or other field-related activities that may affect the data quality of the environmental sample before the sample is received in the laboratory. EPA has established six primary analytical DQOs for environmental studies: precision, accuracy, representativeness, completeness, comparability, and detectability.

The components of analytical variability (uncertainty) can be estimated when QA and QC samples of the right types and quantities are incorporated into measurement procedures at the analytical laboratory. TestAmerica West Sacramento incorporates numerous QA and QC samples to obtain data for comparison with the analytical DQOs and to ensure that the measurement system is functioning properly. The QA and QC samples and their applications, described in Section 8.4 and are selected on the basis of method- or client-specific requirements. Field blanks, field duplicates, and performance evaluation (PE) samples are received from the client as unknown samples. Analytical laboratory QC samples for inorganic, organic, and radionuclide analyses may include calibration or instrument blanks, method blanks, background, duplicates, replicates, laboratory control samples (LCSs), calibration standards, matrix spikes (MSs), matrix spike duplicates (MSDs), surrogate spikes, and yield tracers.

**Data Reduction:**

The process of transforming raw data by arithmetic or statistical calculations, standard curves, concentration factors, etc., and collation into a more useable form. (EPA-QAD)

**Deficiency:**

An unauthorized deviation from acceptable procedures or practices, or a defect in an item. (ASQC)

**Detection Limit:**

The lowest concentration or amount of the target analyte that can be identified, measured, and reported with confidence that the analyte concentration is not a false positive value. See Method Detection Limit. (NELAC)

**Document Control:**

The act of ensuring that documents (and revisions thereto) are proposed, reviewed for accuracy, approved for release by authorized personnel, distributed properly, and controlled to ensure use of the correct version at the location where the prescribed activity is performed. (ASQC)

**Duplicate Analyses:**

The analyses or measurements of the variable of interest performed identically on two subsamples of the same sample. The results from duplicate analyses are used to evaluate analytical or measurement precision but not the precision of sampling, preservation or storage internal to the laboratory. (EPA-QAD)

**Environmental Detection Limit (EDL):**

The smallest level at which a radionuclide in an environmental medium can be unambiguously distinguished for a given confidence interval using a particular combination of sampling and measurement procedures, sample size, analytical detection limit, and processing procedure. The EDL shall be specified for the 0.95 or greater confidence interval. The EDL shall be established initially and verified annually for each test method and sample matrix. (NELAC Radioanalysis Subcommittee)

**Equipment Blank:**

Sample of analyte-free media which has been used to rinse common sampling equipment to check effectiveness of decontamination procedures. (NELAC)

**External Standard Calibration:**

Calibrations for methods that do not utilize internal standards to compensate for changes in instrument conditions.

**Federal Insecticide, Fungicide and Rodenticide Act (FIFRA):**

The enabling legislation under 7 U.S.C. 135 et seq., as amended, that empowers the EPA to register insecticides, fungicides, and rodenticides. (NELAC)

**Federal Water Pollution Control Act (Clean Water Act, CWA):**

The enabling legislation under 33 U.S.C. 1251 et seq., Public Law 92-50086 Stat 816, that empowers EPA to set discharge limitations, write discharge permits, monitor, and bring enforcement action for non-compliance. (NELAC)

**Field Blank:**

Blank prepared in the field by filling a clean container with pure de-ionized water and appropriate preservative, if any, for the specific sampling activity being undertaken (EPA OSWER)

**Field of Testing:**

NELAC's approach to accrediting laboratories by program, method and analyte. Laboratories requesting accreditation for a program-method-analyte combination or for an up-dated/improved method are required to submit to only that portion of the accreditation process not previously addressed (see NELAC, section 1.9ff). (NELAC)

**Finding:**

An assessment conclusion that identifies a condition having a significant effect on an item or activity. As assessment finding is normally a deficiency and is normally accompanied by specific examples of the observed condition. (NELAC)

**Holding Times (Maximum Allowable Holding Times):**

The maximum times that samples may be held prior to analyses and still be considered valid or not compromised. (40 CFR Part 136)

**Inspection:**

An activity such as measuring, examining, testing, or gauging one or more characteristics of an entity and comparing the results with specified requirements in order to establish whether conformance is achieved for each characteristic. (ANSI/ASQC E4-1994)

**Internal Standard:**

A known amount of standard added to a test portion of a sample and carried through the entire measurement process as a reference for evaluating and controlling the precision and bias of the applied analytical test method. (NELAC)

**Internal Standard Calibration:**

Calibrations for methods that utilize internal standards to compensate for changes in instrument conditions.

**Instrument Blank:**

A clean sample (e.g., distilled water) processed through the instrumental steps of the measurement process; used to determine instrument contamination. (EPA-QAD)

**Instrument Response:**

Instrument response is normally expressed as either peak area or peak height however it may also reflect a numerical representation of some type of count on a detector (e.g. Photomultiplier tube, or Diode array detector) and is used in this document to represent all types.

**Laboratory:**

A defined facility performing environmental analyses in a controlled and scientific manner. (NELAC)

**Laboratory Control Sample (however named, such as laboratory fortified blank, spiked blank, or QC check sample):**

A sample matrix, free from the analytes of interest, spiked with verified known amounts of analytes or a material containing known and verified amounts of analytes, taken through all preparation and analysis steps. Where there is no preparation taken for an analysis (such as in aqueous volatiles), or when all samples and standards undergo the same preparation and analysis process (such as Phosphorus), there is no LCS. It is generally used to establish intra-laboratory or analyst specific precision and bias or to assess the performance of all or a portion of the measurement system.

An LCS shall be prepared at a minimum of 1 per batch of 20 or less samples per matrix type per sample extraction or preparation method except for analytes for which spiking solutions are not available such as total suspended solids, total dissolved solids, total volatile solids, total solids, pH, color, odor, temperature, dissolved oxygen or turbidity. The results of these samples shall be used to determine batch acceptance.

Note: NELAC standards allow a matrix spike to be used in place of this control as long as the acceptance criteria are as stringent as for the LCS. (NELAC)

**Laboratory Duplicate:**

Aliquots of a sample taken from the same container under laboratory conditions and processed and analyzed independently. (NELAC)

**Least Squares Regression (1<sup>st</sup> Order Curve):**

The least squares regression is a mathematical calculation of a straight line over two axes. The y axis represents the instrument response (or Response ratio) of a standard or sample and the x axis represents the concentration. The regression calculation will generate a correlation coefficient (r) that is a measure of the "goodness of fit" of the regression line to the data. A value of 1.00 indicates a perfect fit. In order to be used for quantitative purposes, r must be greater than or equal to 0.99 for organics and 0.995 for inorganics.

**Limit of Detection (LOD):**

An estimate of the minimum amount of a substance that an analytical process can reliably detect. An LOD is analyte- and matrix-specific and may be laboratory dependent. (Analytical Chemistry, 55, p.2217, December 1983, modified) See also Method Detection Limit.

**Manager (however named):**

The individual designed as being responsible for the overall operation, all personnel, and the physical plant of the environmental laboratory. A supervisor may report to the manager. In some cases, the supervisor and the manager may be the same individual. (NELAC)

**Matrix:**

The component or substrate that contains the analyte of interest. For purposes of batch and QC requirement determinations, the following matrix distinctions shall be used:

**Aqueous:** Any aqueous sample excluded from the definition of Drinking Water matrix or Saline/Estuarine source. Includes surface water, groundwater, effluents, and TCLP or other extracts.

**Drinking Water:** any aqueous sample that has been designated as a potable or potential potable water source.

**Saline/Estuarine:** any aqueous sample from an ocean or estuary, or other salt water source such as the Great Salt Lake.

**Non-aqueous Liquid:** any organic liquid with <15% settleable solids.

**Biological Tissue:** any sample of a biological origin such as fish tissue, shellfish, or plant material. Such samples shall be grouped according to origin.

**Solids:** includes soils, sediments, sludges, and other matrices with >15% settleable solids.

**Chemical Waste:** a product or by-product of an industrial process that results in a matrix not previously defined.

**Air:** whole gas or vapor samples including those contained in flexible or rigid wall containers and the extracted concentrated analytes of interest from a gas or vapor that are collected with a sorbant tube, impinger solution, filter, or other device. (NELAC)

**Matrix Spike (spiked sample or fortified sample):**

Prepared by adding a known mass of target analyte to a specified amount of matrix sample for which an independent estimate of target analyte concentration is available. Matrix spikes are used, for example, to determine the effect of the matrix on a method's recovery efficiency.

Matrix spikes shall be performed at a frequency of one in 20 samples per matrix type per sample extraction or preparation method except for analytes for which spiking solutions are not available such as, total suspended solids, total dissolved solids, total volatile solids, total solids, pH, color, odor, temperature, dissolved oxygen or turbidity. The selected sample(s) shall be rotated among client samples so that various matrix problems may be noted and/or addressed. Poor performance in a matrix spike may indicate a problem with the sample composition and shall be reported to the client whose sample was used for the spike. (QAMS)

**Matrix Spike Duplicate (spiked sample or fortified sample duplicate):**

A second replicate matrix spike is prepared in the laboratory and analyzed to obtain a measure of the precision of the recovery for each analyte.

Matrix spike duplicates or laboratory duplicates shall be analyzed at a minimum of 1 in 20 samples per matrix type per sample extraction or preparation method. The laboratory shall document their procedure to select the use of an appropriate type of duplicate. The selected sample(s) shall be rotated among client samples so that various matrix problems may be noted and/or addressed. Poor performance in the duplicates may indicate a problem with the sample composition and shall be reported to the client whose sample was used for the duplicate. (QAMS)

**Method Blank:**

A sample of a matrix similar to the batch of associated samples (when available) that is free from the analytes of interest and is processed simultaneously with and under the same conditions as samples through all steps of the analytical procedures, and in which no target analytes or interferences are present at concentrations that impact the analytical results for sample analyses. (NELAC)

**Method Detection Limit:**

The minimum concentration of a substance (an analyte) that can be measured and reported with 99% confidence that the analyte concentration is greater than zero and is determined from analysis of a sample in a given matrix containing the analyte. (40 CFR Part 136, Appendix B)

**National Environmental Laboratory Accreditation Conference (NELAC):**

A voluntary organization of State and Federal environmental officials and interest groups purposed primarily to establish mutually acceptable standards for accrediting environmental laboratories. A subset of NELAP. (NELAC)

**National Environmental Laboratory Accreditation Program (NELAP):**

The overall National Environmental Laboratory Accreditation Program of which NELAC is a part. (NELAC)

**Negative Control:**

Measures taken to ensure that a test, its components, or the environment do not cause undesired effects, or produce incorrect test results. (NELAC)

**NELAC Standards:**

The plan of procedures for consistently evaluating and documenting the ability of laboratories performing environmental measurements to meet nationally defined standards established by the National Environmental Laboratory Accreditation Conference. (NELAC)

*Outlier:*

*A result excluded from the statistical calculations due to being deemed "suspicious" when applying the "Grubbs Test" (or equivalent).*

**Performance Audit:**

The routine comparison of independently obtained qualitative and quantitative measurement system data with routinely obtained data in order to evaluate the proficiency of an analyst or laboratory. (NELAC)

**Performance Based Measurement System (PBMS):**

A set of processes wherein the data quality needs, mandates or limitations of a program or project are specified and serve as criteria for selecting appropriate test methods to meet those needs in a cost-effective manner. (NELAC)

**Positive Control:**

Measures taken to ensure that a test and/or its components are working properly and producing correct or expected results from positive test subjects. (NELAC)

**Precision:**

The degree to which a set of observations or measurements of the same property, obtained under similar conditions, conform to themselves; a data quality indicator. Precision is usually expressed as standard deviation, variance or range, in either absolute or relative terms. (NELAC)

**Preservation:**

Refrigeration and/or reagents added at the time of sample collection (or later) to maintain the chemical and/or biological integrity of the sample. (NELAC)

**Proficiency Testing:**

A means of evaluating a laboratory's performance under controlled conditions relative to a given set of criteria through analysis of unknown samples provided by an external source. (NELAC)  
[2.1]

**Proficiency Testing Program:**

The aggregate of providing rigorously controlled and standardized environmental samples to a laboratory for analysis, reporting of results, statistical evaluation of the results and the collective demographics and results summary of all participating laboratories. (NELAC)

**Proficiency Test Sample (PT):**

A sample, the composition of which is unknown to the analyst and is provided to test whether the analyst/laboratory can produce analytical results within specified acceptance criteria. (QAMS)

**Quality Assurance:**

An integrated system of activities involving planning, quality control, quality assessment, reporting and quality improvement to ensure that a product or service meets defined standards of quality with a stated level of confidence. (QAMS)

**Quality Assurance [Project] Plan (QAPP):**

A formal document describing the detailed quality control procedures by which the quality requirements defined for the data and decisions pertaining to a specific project are to be achieved. (EAP-QAD)

**Quality Control:**

The overall system of technical activities which purpose is to measure and control the quality of a product or service so that it meets the needs of users. (QAMS)

**Quality Control Sample:**

An uncontaminated sample matrix spiked with known amounts of analytes from a source independent from the calibration standards. It is generally used to establish intra-laboratory or analyst specific precision and bias or to assess the performance of all or a portion of the measurement system. (EPA-QAD)

**Quality Manual:**

A document stating the management policies, objectives, principles, organizational structure and authority, responsibilities, accountability, and implementation of an agency, organization, or laboratory, to ensure the quality of its product and the utility of its product to its users. (NELAC)

**Quality System:**

A structured and documented management system describing the policies, objectives, principles, organizational authority, responsibilities, accountability, and implementation plan of an organization for ensuring quality in its work processes, products (items), and services. The quality system provides the framework for planning, implementing, and assessing work performed by the organization and for carrying out required QA and QC (ANSI/ASQC-E-41994)

**Quantitation Limits:**

The maximum or minimum levels, concentrations, or quantities of a target variable (e.g., target analyte) that can be quantified with the confidence level required by the data user. (NELAC)

**Range:**

The difference between the minimum and the maximum of a set of values. (EPA-QAD)

**Reagent Blank (method reagent blank):**

A sample consisting of reagent(s), without the target analyte or sample matrix, introduced into the analytical procedure at the appropriate point and carried through all subsequent steps to determine the contribution of the reagents and of the involved analytical steps. (QAMS)

**Reference Material:**

A material or substance one or more properties of which are sufficiently well established to be used for the calibration of an apparatus, the assessment of a measurement method, or for assigning values to materials. (ISO Guide 30-2.1)

**Reference Method:**

A method of known and documented accuracy and precision issued by an organization recognized as competent to do so. (NELAC)

**Reference Standard:**

A standard, generally of the highest metrological quality available at a given location, from which measurements made at that location are derived. (VIM-6.0-8)

**Replicate Analyses:**

The measurements of the variable of interest performed identically on two or more sub-samples of the same sample within a short time interval. (NELAC)

**Representativeness:**

Representativeness is the degree to which data accurately and precisely represent a characteristic of a population, a variation in a physical or chemical property at a sampling point, or an environmental condition. Data representativeness is primarily a function of sampling strategy; therefore, the sampling scheme must be designed to maximize representativeness. Representativeness also relates to ensuring that, through sample homogeneity, the sample analysis result (concentration) is representative of the constituent concentration in the sample matrix. At each TestAmerica laboratory, every effort must be made to analyze an aliquot that is representative of the original sample, and to ensure the homogeneity of the sample before subsampling.

**Requirement:**

Denotes a mandatory specification; often designated by the term "shall". (NELAC)

**Resource Conservation and Recovery Act (RCRA):**

The enabling legislation under 42 USC 321 et seq. (1976), that gives EPA the authority to control hazardous waste from the "cradle-to-grave", including its generation, transportation, treatment, storage, and disposal. (NELAC)

**Safe Drinking Water Act (SDWA):**

The enabling legislation, 42 USC 300f et seq. (1974), (Public Law 93-523), that requires the EPA to protect the quality of drinking water in the U.S. by setting maximum allowable contaminant levels, monitoring, and enforcing violations. (NELAC)

**Sample Duplicate:**

Two samples taken from and representative of the same population and carried through all steps of the sampling and analytical procedures in an identical manner. Duplicate samples are used to assess variance of the total method including sampling and analysis. (EPA-QAD)

**Second Order Polynomial Curve (Quadratic):**

The 2<sup>nd</sup> order curves are a mathematical calculation of a slightly curved line over two axes. The y axis represents the instrument response (or Response ratio) of a standard or sample and the x axis represents the concentration. The 2<sup>nd</sup> order regression will generate a coefficient of determination (COD or  $r^2$ ) that is a measure of the "goodness of fit" of the quadratic curvature the data. A value of 1.00 indicates a perfect fit. In order to be used for quantitative purposes,  $r^2$  must be greater than or equal to 0.99.

**Selectivity:**

(Analytical chemistry) the capability of a test method or instrument to respond to a target substance of constituent in the presence of non-target substances. (EPA-QAD)

**Sensitivity:**

The capability of a method or instrument to discriminate between measurement responses representing different levels (e.g., concentrations) of a variable of interest. (NELAC)

**Spike:**

A known mass of target analyte added to a blank, sample or sub-sample; used to determine recovery efficiency or for other quality control purposes.

If the mandated or requested test method does not specify the spiking components, the laboratory shall spike all reportable components to be reported in the Laboratory Control Sample and Matrix Spike. However, in cases where the components interfere with accurate assessment (such as simultaneously spiking chlordane, toxaphene and PCBs in Method 608), the test method has an extremely long list of components or components are incompatible, a representative number (at a minimum 10%) of the listed components may be used to control the test method. The selected components of each spiking mix shall represent all chemistries, elution patterns and masses permit specified analytes and other client requested components. However, the laboratory shall ensure that all reported components are used in the spike mixture within a two-year time period. (NELAC)

**Standard:**

The document describing the elements of laboratory accreditation that has been developed and established within the consensus principles of NELAC and meets the approval requirements of NELAC procedures and policies. (ASQC)

**Standard Operating Procedures (SOPs):**

A written document which details the method of an operation, analysis, or action whose techniques and procedures are thoroughly prescribed and which is accepted as the method for performing certain routine or repetitive tasks. (QAMS)

**Standardized Reference Material (SRM):**

A certified reference material produced by the U.S. National Institute of Standards and Technology or other equivalent organization and characterized for absolute content, independent of analytical method. (EPA-QAD)

**Supervisor (however named):**

The individual(s) designated as being responsible for a particular area or category of scientific analysis. This responsibility includes direct day-to-day supervision of technical employees, supply and instrument adequacy and upkeep, quality assurance/quality control duties, and ascertaining that technical employees have the required balance of education, training and experience to perform the required analyses. (NELAC)

**Surrogate:**

A substance with properties that mimic the analyte of interest. It is unlikely to be found in environment samples and is added to them for quality control purposes.

Surrogate compounds must be added to all samples, standards, and blanks, for all organic chromatography methods except when the matrix precludes its use or when a surrogate is not available. Poor surrogate recovery may indicate a problem with sample composition and shall be reported to the client whose sample produced poor recovery. (QAMS)

**Systems Audit (also Technical Systems Audit):**

A thorough, systematic, qualitative on-site assessment of the facilities, equipment, personnel, training, procedures, record keeping, data validation, data management, and reporting aspects of a total measurement system. (EPA-QAD)

**Technical Director:**

Individual(s) who has overall responsibility for the technical operation of the environmental testing laboratory. (NELAC)

**Test:**

A technical operation that consists of the determination of one or more characteristics or performance of a given product, material, equipment, organism, physical phenomenon, process, or service according to a specified procedure. The result of a test is normally recorded in a document sometimes called a test report or a test certificate. (ISO/IEC Guide 2-12.1, amended)

**Test Method:**

An adoption of a scientific technique for a specific measurement problem, as documented in a laboratory SOP. (NELAC)

**Toxic Substances Control Act (TSCA):**

The enabling legislation in 15 USC 2601 et seq., (1976) that provides for testing, regulating, and screening all chemicals produced or imported into the United States for possible toxic effects prior to commercial manufacture. (NELAC)

**Traceability:**

The property of a result of a measurement whereby it can be related to appropriate standards, generally international or national standards, through an unbroken chain of comparisons. (VIM-6.12)

**Uncertainty:**

A parameter associated with the result of a measurement that characterizes the dispersion of the value that could reasonably be attributed to the measured value.

**United States Environmental Protection Agency (EPA):**

The Federal governmental agency with responsibility for protecting public health and safeguarding and improving the natural environment (i.e., the air, water, and land) upon which human life depends. (US-EPA)

**Validation:**

The process of substantiating specified performance criteria. (EPA-QAD)

**Verification:**

Confirmation by examination and provision of evidence that specified requirements have been met. (NELAC)

**NOTE:** In connection with the management of measuring equipment, verification provides a means for checking that the deviations between values indicated by a measuring instrument and corresponding known values of a measured quantity are consistently smaller than the maximum allowable error defined in a standard, regulation or specification peculiar to the management of the measuring equipment.

The result of verification leads to a decision either to restore in service, to perform adjustment, to repair, to downgrade, or to declare obsolete. In all cases, it is required that a written trace of the verification performed shall be kept on the measuring instrument's individual record.

**Work Cell:**

A well-defined group of analysts that together perform the method analysis. The members of the group and their specific functions within the work cell must be fully documented. (NELAC)

**Acronyms:**

A2LA – American Association for Laboratory Accreditation  
ANSI – American National Standards Institute  
ASQ – American Society for Quality  
ASTM – American Society for Testing and Materials  
BS – Blank Spike  
BSD – Blank Spike Duplicate  
CAR – Corrective Action Report  
CCB – Continuing Calibration Blank  
CCC – Calibration Check Compound  
CCV – Continuing Calibration Verification  
CERCLA – Comprehensive Environmental Response, Compensation and Liability Act  
CF – Calibration Factor  
CFR – Code of Federal Regulations  
CLP – Contract Laboratory Program  
COC – Chain of Custody  
CRS – Change Request Form  
DOC – Demonstration of Capability  
DOD – Department of Defence  
DQO – Data Quality Objectives  
DU – Duplicate  
DUP - Duplicate  
EHS – Environment, Health and Safety  
EPA – Environmental Protection Agency  
GC - Gas Chromatography  
GC/MS - Gas Chromatography/Mass Spectrometry  
HPLC - High Performance Liquid Chromatography  
ICP - Inductively Coupled Plasma Atomic Emission Spectroscopy  
ICB – Initial Calibration Blank  
ICV – Initial Calibration Verification  
IDL – Instrument Detection Limit  
IH – Industrial Hygiene  
IS – Internal Standard  
ISO – International Standards Organization  
LCS – Laboratory Control Sample  
LCSD – Laboratory Control Sample Duplicate  
LIMS – Laboratory Information Management System  
MDL – Method Detection Limit  
MS – Matrix Spike  
MSD – Matrix Spike Duplicate  
MSDS - Material Safety Data Sheet  
NELAC - National Environmental Laboratory Accreditation Conference  
NELAP - National Environmental Laboratory Accreditation Program  
NIOSH – National Institute for Occupational Safety and Health  
NPDES – National Pollutant Discharge Elimination System  
NRC – Nuclear Regulatory Commission  
NRM – National Reference Material  
PT – Performance Testing  
PUF – Polyurethane Foam  
QAM – Quality Assurance Manual

QA/QC – Quality Assurance / Quality Control  
QAPP – Quality Assurance Project Plan  
RCRA – Resource Conservation and Recovery Act  
RF – Response Factor  
RPD – Relative Percent Difference  
RSD – Relative Standard Deviation  
SD – Standard Deviation  
SOP – Standard Operating Procedure  
SPCC – System Performance Check Compound  
TAT – Turn-Around-Time  
VOA – Volatiles  
VOC – Volatile Organic Compound  
WS – Water Supply  
WP – Water Pollution

**Appendix 6.**

**Laboratory Certifications, Accreditations, Validations**

TestAmerica West Sacramento maintains certifications, accreditations, certifications, and validations with numerous state and national entities. Programs vary but may include on-site audits, reciprocal agreements with another entity, performance testing evaluations, review of the QA Manual, Standard Operating Procedures, Method Detection Limits, training records, etc. At the time of this QA Manual revision, the laboratory has accreditation/certification/licensing with the following organizations:

Organization	Certificate Number Or Laboratory ID Number	Organization	Certificate Number Or Laboratory ID Number
AFCEE	--	Nevada	CA44
Alaska	UST-055	New Jersey	CA005
Arizona	AZ0616	New York	11666
Arkansas	88-0691	Oregon	CA200005
California	01119CA	Pennsylvania	68-01272
Colorado	--	South Carolina	87014002
Connecticut	PH-0691	Texas	TX270-2007B
EPA - UCMR	--	Utah	QUAN1
EPA – UCMR2	--	USACE	--
Florida	E87570	USDA Soil Permit	S-73787
Georgia	960	Virginia	00178
Hawaii	--	Washington	C1281
Kansas	E-10375	West Virginia (DOH)	9930C
Louisiana	01944	West Virginia (DEP)	334
Michigan	9947	Wisconsin	998204680
NFESC (Navy)	--		

The certificates and parameter lists (which may differ) for each organization may be found on the corporate web site, the laboratory’s public server, the final report review table, and in the QA office.

**Claims of Accreditation Status**

TestAmerica West Sacramento has agreed to make only valid claims as to its accreditation/certification status by any authority by ensuring that the expiration dates are not exceeded and the method-specific scope or parameter lists are supportable, as required by each. Any false claims would be reported to that authority. The agreement covers the use of the authority’s name, such as “Authority-Accredited,” logo, or certificate number. The only valid proof of accreditation/certification is the current certificate and scope of the authority. It is the responsibility of the laboratory to make these documents available to all staff, and it is the staff’s duty to reference only the current documents.

**Appendix 7. Data Qualifiers**

<b>Qualifier Organic</b>	<b>Qualifier Inorganic</b>	<b>Footnote</b>
<b>U</b>	<b>U</b>	<b>Analyte analyzed for but was not detected.</b>
<b>G</b>	<b>G</b>	<b>Elevated reporting limit. The reporting limit is elevated due to matrix interference.</b>
<b>J</b>	<b>B</b>	<b>Estimated result. Result is less than RL.</b>
<b>E</b>	<b>I</b>	<b>Estimated result. Result concentration exceeds the calibration range.</b>
<b>B</b>	<b>J</b>	<b>Method blank contamination. The associated method blank contains the target analyte at a reportable level.</b>
<b>P</b>	<b>*</b>	<b>Relative percent difference (RPD) is outside stated control limits.</b>
<b>a</b>	<b>N</b>	<b>Spiked analyte recovery is outside stated control limits.</b>
<b>*</b>		<b>Surrogate recovery is outside stated control limits.</b>
<b>PG</b>		<b>The percent difference between the original and confirmation analyses is greater than 40%.</b>

**This is not an all-inclusive list of qualifiers. All qualifiers are defined on each data sheet. Client specific qualifiers may also be used, and would also be defined on the data sheet.**